

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
 Data File : VV023295.D
 Acq On : 09 Nov 2021 11:36
 Operator : SY/MD
 Sample : M4445-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG381

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023295.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	93	rVB	57036	57836	12.82%	1.510%
2	1.568	156	164	176	rBV	53543	60335	13.37%	1.575%
3	1.632	177	184	194	rVB4	4713	7211	1.60%	0.188%
4	2.108	322	332	345	rBV	96410	136373	30.22%	3.560%
5	2.179	345	354	371	rVB2	6242	15813	3.50%	0.413%
6	2.507	446	456	470	rVB2	12908	22941	5.08%	0.599%
7	3.044	614	623	634	rVB9	2991	5959	1.32%	0.156%
8	3.889	875	886	937	rBV	43455	149941	33.23%	3.915%
9	4.346	1011	1028	1049	rBV3	74401	189148	41.92%	4.938%
10	4.677	1118	1131	1141	rBV6	2165	4892	1.08%	0.128%
11	5.044	1229	1245	1282	rBV3	160591	451242	100.00%	11.781%
12	5.616	1411	1423	1452	rBV	139621	293558	65.06%	7.664%
13	6.066	1549	1563	1589	rBV2	94252	203059	45.00%	5.301%
14	6.986	1836	1849	1867	rBV2	44005	82834	18.36%	2.163%
15	7.317	1939	1952	1966	rBV	179346	317423	70.34%	8.287%
16	7.387	1966	1974	1996	rVB	51275	96801	21.45%	2.527%
17	7.625	2039	2048	2061	rBV	25925	46572	10.32%	1.216%
18	8.088	2182	2192	2229	rBV	179958	350529	77.68%	9.151%
19	8.252	2239	2243	2260	rVB7	3534	6132	1.36%	0.160%
20	8.850	2418	2429	2455	rBV	220871	371264	82.28%	9.693%
21	9.018	2472	2481	2493	rBV	8336	13753	3.05%	0.359%
22	9.140	2508	2519	2537	rBV2	25563	43558	9.65%	1.137%
23	9.545	2634	2645	2657	rBV	24411	38070	8.44%	0.994%
24	10.217	2843	2854	2866	rBV	64839	103318	22.90%	2.697%
25	10.452	2915	2927	2943	rVV2	6958	13313	2.95%	0.348%
26	10.542	2944	2955	2964	rVB2	5143	7408	1.64%	0.193%
27	10.741	3008	3017	3026	rVB3	4539	6645	1.47%	0.173%
28	10.915	3062	3071	3090	rVB	18771	28894	6.40%	0.754%
29	11.249	3164	3175	3194	rBV	232094	356728	79.05%	9.313%
30	11.339	3195	3203	3212	rVB2	9035	14110	3.13%	0.368%
31	11.532	3253	3263	3274	rBV7	9671	17601	3.90%	0.460%
32	11.625	3280	3292	3310	rVB	186649	300275	66.54%	7.839%
33	12.345	3507	3516	3524	rBV5	8877	11841	2.62%	0.309%
34	12.882	3676	3683	3692	rVB5	3785	4937	1.09%	0.129%

Sum of corrected areas: 3830314




Instrument :
MSVOA_V
ClientSampleId :
BG381

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023295.D
Acq On : 09 Nov 2021 11:36
Operator : SY/MD
Sample : M4445-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG381

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

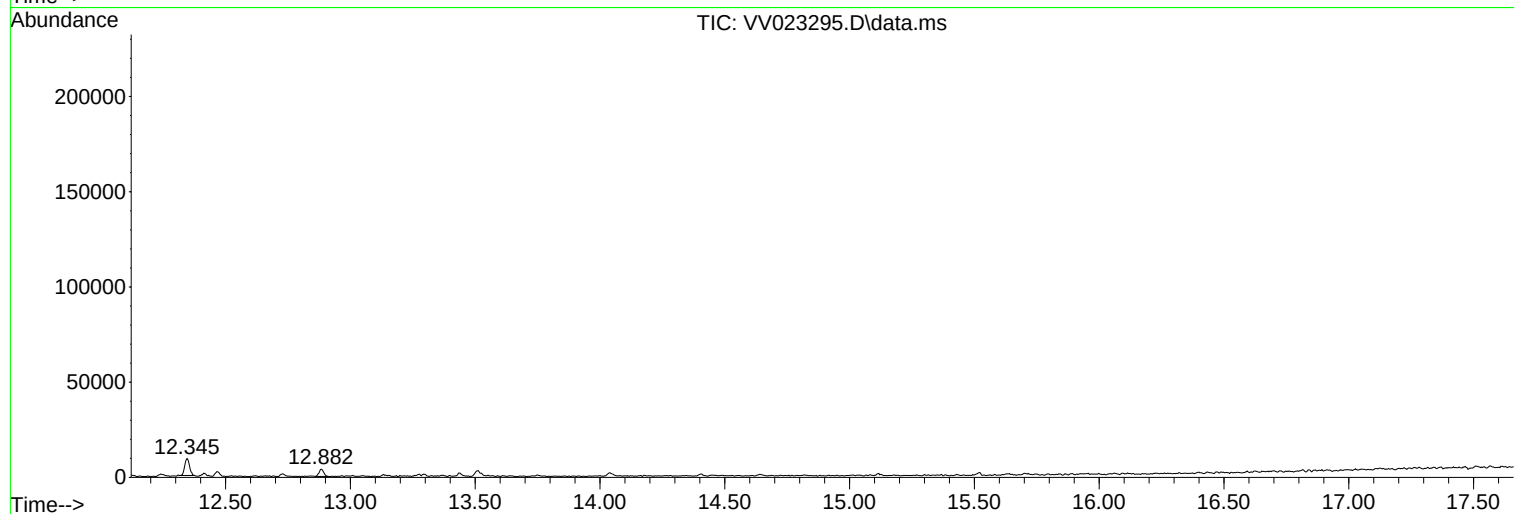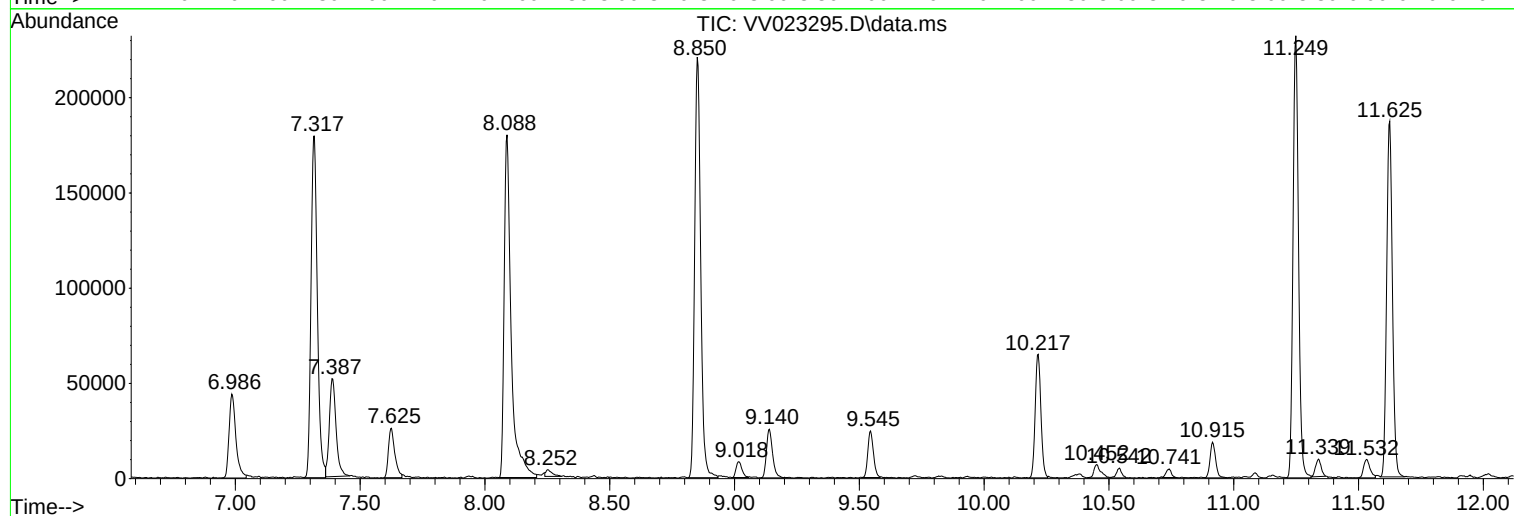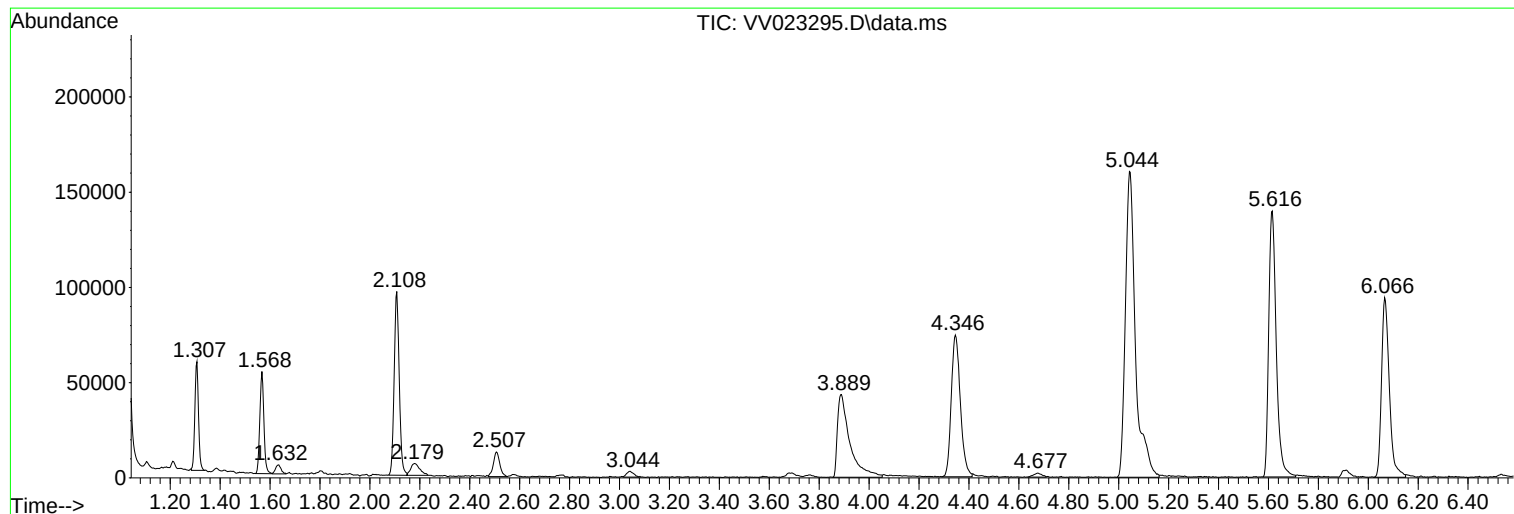

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023295.D
Acq On : 09 Nov 2021 11:36
Operator : SY/MD
Sample : M4445-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG381

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023295.D
Acq On : 09 Nov 2021 11:36
Operator : SY/MD
Sample : M4445-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG381

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc