

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
 Data File : VV023303.D
 Acq On : 09 Nov 2021 15:13
 Operator : SY/MD
 Sample : M4558-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB883

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023303.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	72	82	95	rVB2	64939	95895	22.32%	2.632%
2	1.568	154	164	176	rBV	54480	62465	14.54%	1.714%
3	2.108	321	332	344	rBV	96269	143233	33.34%	3.931%
4	2.175	344	353	369	rVB2	8847	19578	4.56%	0.537%
5	3.886	874	885	922	rBV	52037	159609	37.15%	4.381%
6	4.349	1013	1029	1052	rBV2	76699	200940	46.78%	5.515%
7	5.047	1231	1246	1281	rBV3	167985	429583	100.00%	11.791%
8	5.619	1412	1424	1450	rBV	147459	307813	71.65%	8.449%
9	5.911	1505	1515	1530	rVB8	4524	10205	2.38%	0.280%
10	6.072	1550	1565	1587	rBV	98818	208695	48.58%	5.728%
11	6.989	1838	1850	1869	rBV	45021	86886	20.23%	2.385%
12	7.317	1939	1952	1968	rBV	187143	329744	76.76%	9.051%
13	7.625	2038	2048	2071	rBV	26227	50713	11.81%	1.392%
14	8.088	2183	2192	2227	rBV	185913	371565	86.49%	10.198%
15	8.853	2417	2430	2448	rBV	237037	386578	89.99%	10.611%
16	10.217	2841	2854	2866	rBV	64988	104581	24.34%	2.870%
17	10.381	2897	2905	2915	rVB4	4246	6290	1.46%	0.173%
18	11.249	3164	3175	3195	rBV	230764	359837	83.76%	9.877%
19	11.538	3254	3265	3273	rBV9	2618	4673	1.09%	0.128%
20	11.625	3281	3292	3313	rBV	195411	304468	70.88%	8.357%




Sum of corrected areas: 3643351

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023303.D
Acq On : 09 Nov 2021 15:13
Operator : SY/MD
Sample : M4558-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB883

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

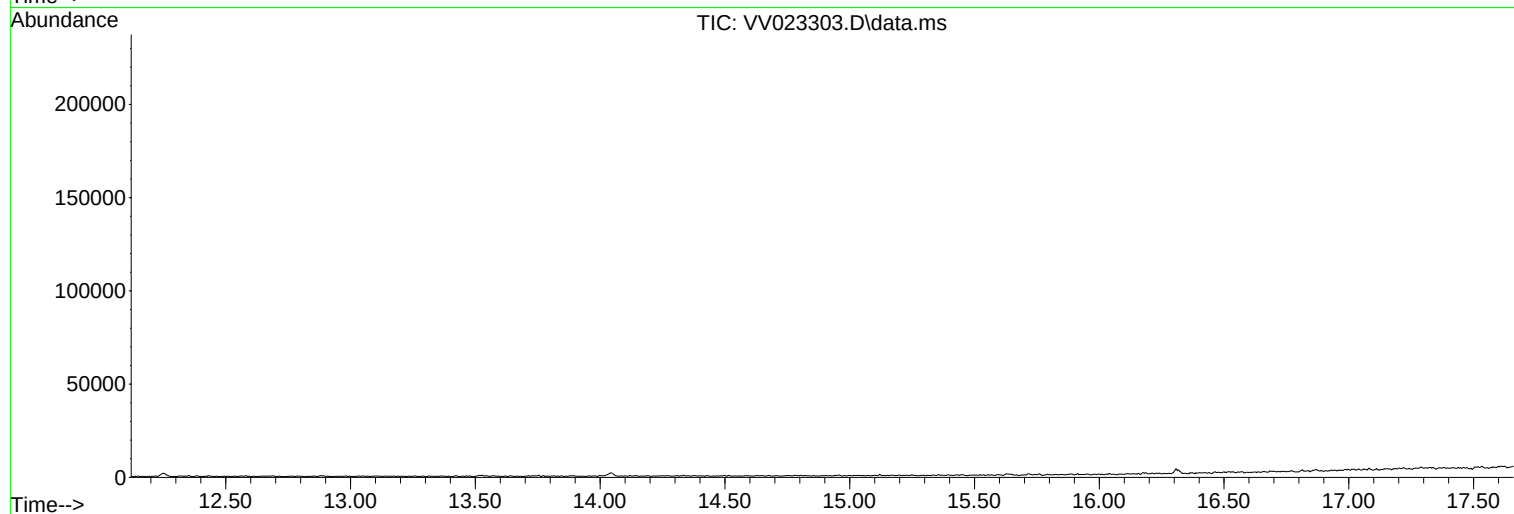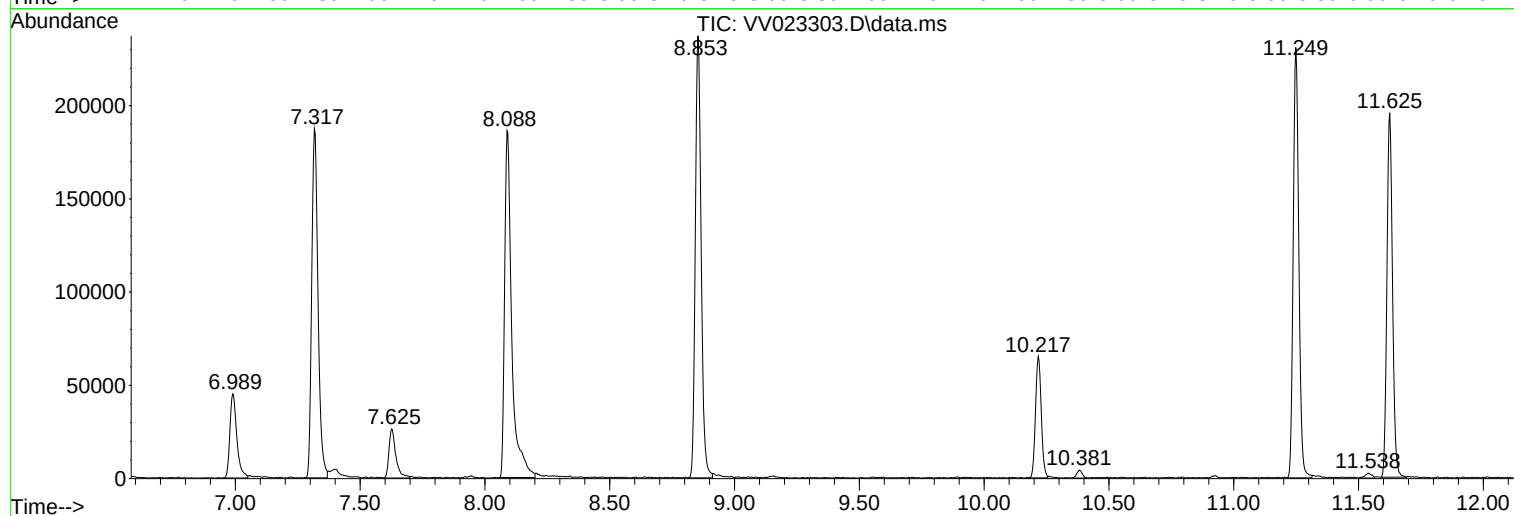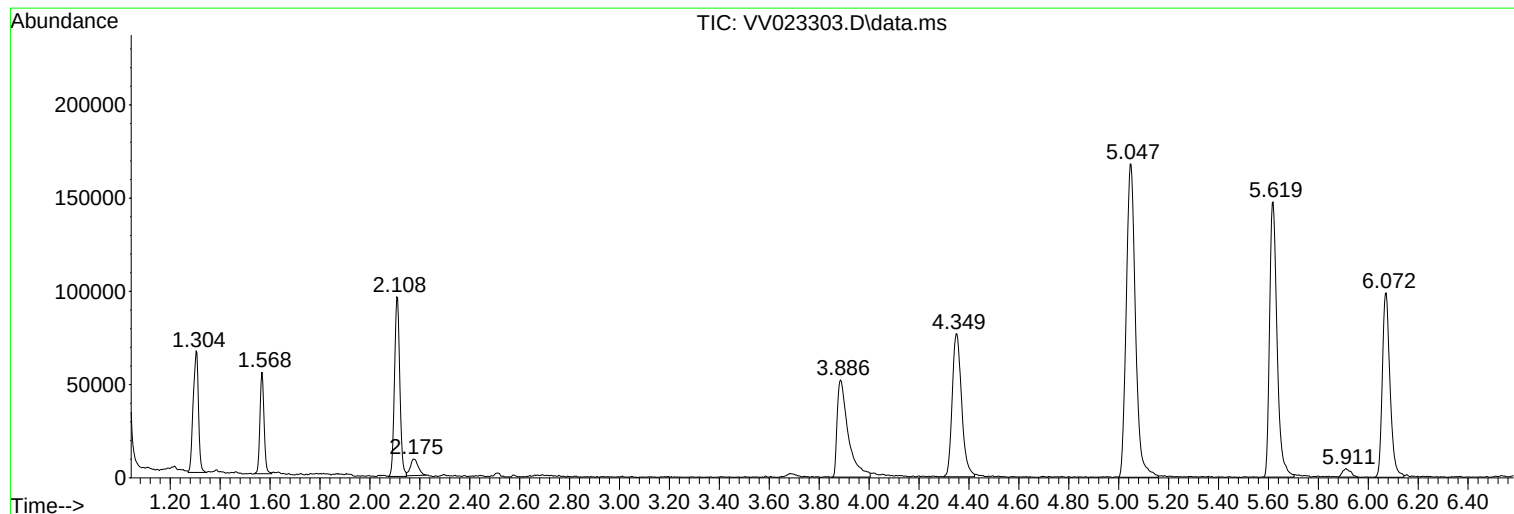

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023303.D
Acq On : 09 Nov 2021 15:13
Operator : SY/MD
Sample : M4558-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB883

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023303.D
Acq On : 09 Nov 2021 15:13
Operator : SY/MD
Sample : M4558-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB883

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc