

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
 Data File : VV023306.D
 Acq On : 09 Nov 2021 16:23
 Operator : SY/MD
 Sample : M4558-24
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB886

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023306.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	95	rVB	51706	54703	13.04%	1.481%
2	1.568	157	164	174	rBV	49661	55639	13.26%	1.507%
3	2.111	321	333	344	rBV	93036	132203	31.50%	3.580%
4	2.179	344	354	385	rVB2	20960	59131	14.09%	1.601%
5	3.896	869	888	931	rBV3	66967	243450	58.01%	6.592%
6	4.352	1015	1030	1054	rBV2	74729	185511	44.21%	5.023%
7	5.050	1232	1247	1270	rBV2	160041	402419	95.90%	10.897%
8	5.619	1412	1424	1455	rBV	160177	330702	78.81%	8.955%
9	5.912	1506	1515	1529	rVB3	4820	9689	2.31%	0.262%
10	6.072	1551	1565	1588	rBV	96321	200383	47.75%	5.426%
11	6.989	1839	1850	1873	rBV2	43796	82612	19.69%	2.237%
12	7.317	1940	1952	1974	rBV	174623	312505	74.47%	8.462%
13	7.628	2039	2049	2065	rBV2	25729	47386	11.29%	1.283%
14	8.091	2179	2193	2227	rBV	179827	363063	86.52%	9.831%
15	8.854	2418	2430	2453	rBV	255157	419645	100.00%	11.363%
16	10.217	2843	2854	2870	rBV	63607	102521	24.43%	2.776%
17	10.384	2894	2906	2917	rVB4	3191	5191	1.24%	0.141%
18	11.249	3165	3175	3199	rBV	250047	386560	92.12%	10.467%
19	11.625	3278	3292	3312	rBV	182670	294241	70.12%	7.968%
20	13.435	3848	3855	3865	rBV6	3715	5414	1.29%	0.147%




Sum of corrected areas: 3692968

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023306.D
Acq On : 09 Nov 2021 16:23
Operator : SY/MD
Sample : M4558-24
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB886

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

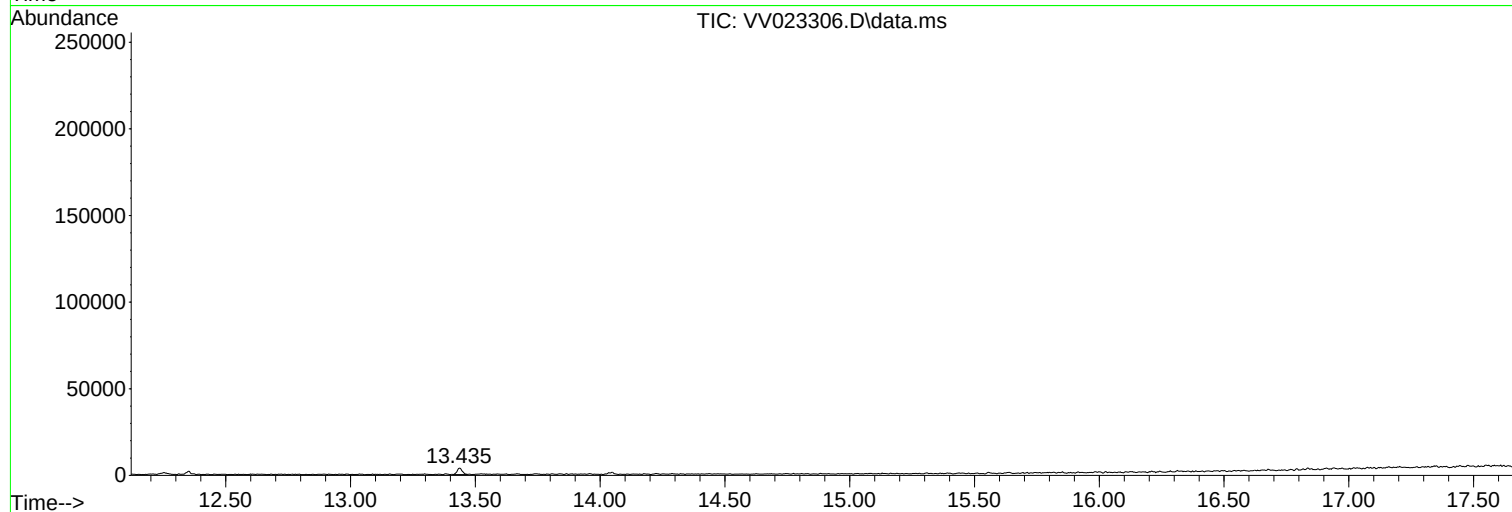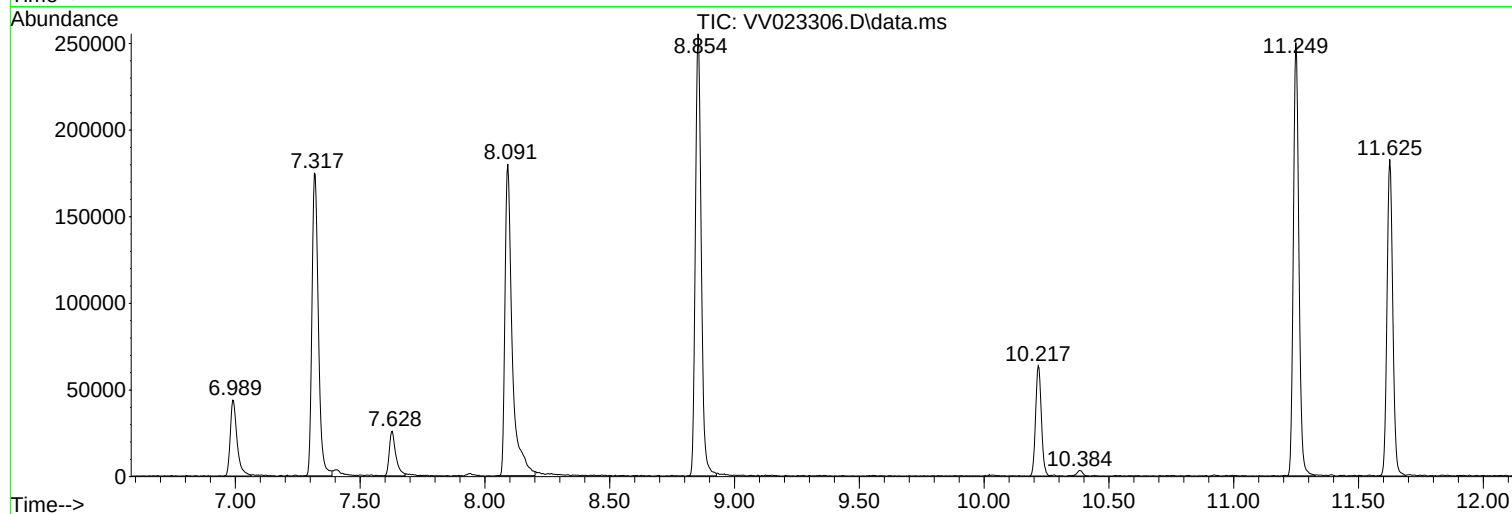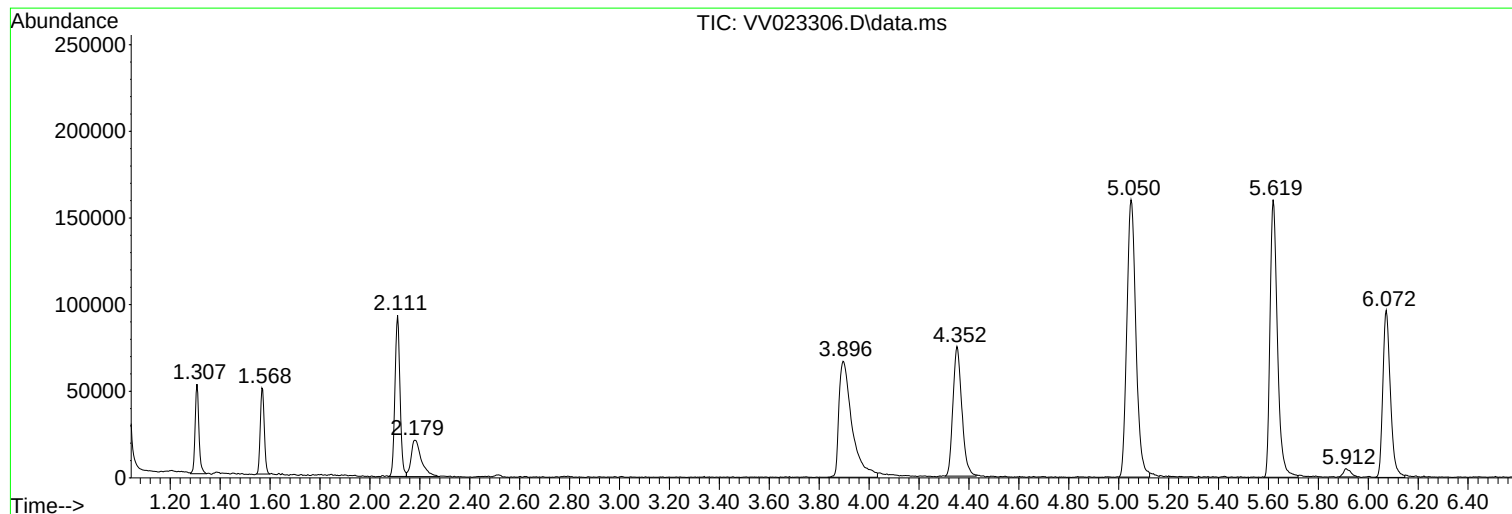

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023306.D
Acq On : 09 Nov 2021 16:23
Operator : SY/MD
Sample : M4558-24
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB886

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023306.D
Acq On : 09 Nov 2021 16:23
Operator : SY/MD
Sample : M4558-24
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB886

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc