

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
 Data File : VV023316.D
 Acq On : 09 Nov 2021 20:17
 Operator : SY/MD
 Sample : M4522-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3A0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023316.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	97	rVB	45556	47795	13.03%	1.516%
2	1.568	157	164	175	rBV	44037	48963	13.35%	1.554%
3	2.108	322	332	345	rBV	80997	116105	31.64%	3.684%
4	3.886	873	885	920	rBV	43594	134850	36.75%	4.279%
5	4.352	1015	1030	1052	rBV	67949	172279	46.96%	5.466%
6	5.050	1230	1247	1274	rBV3	144580	366899	100.00%	11.641%
7	5.619	1412	1424	1451	rBV	137723	284020	77.41%	9.012%
8	5.912	1508	1515	1532	rVB4	2465	4916	1.34%	0.156%
9	6.072	1553	1565	1585	rBV	88881	182867	49.84%	5.802%
10	6.989	1840	1850	1870	rBV2	38710	74196	20.22%	2.354%
11	7.317	1941	1952	1973	rBV	159766	285463	77.80%	9.057%
12	7.407	1975	1980	1991	rVB8	2913	4702	1.28%	0.149%
13	7.629	2040	2049	2064	rBV2	23690	42377	11.55%	1.345%
14	8.092	2182	2193	2229	rBV	169368	332298	90.57%	10.543%
15	8.442	2291	2302	2310	rBV5	2945	4867	1.33%	0.154%
16	8.854	2417	2430	2448	rBV	220438	358868	97.81%	11.386%
17	10.217	2843	2854	2870	rBV	63707	101222	27.59%	3.212%
18	11.249	3165	3175	3194	rBV	210817	325135	88.62%	10.316%
19	11.625	3281	3292	3311	rBV	167337	263886	71.92%	8.373%




Sum of corrected areas: 3151708

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023316.D
Acq On : 09 Nov 2021 20:17
Operator : SY/MD
Sample : M4522-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3A0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

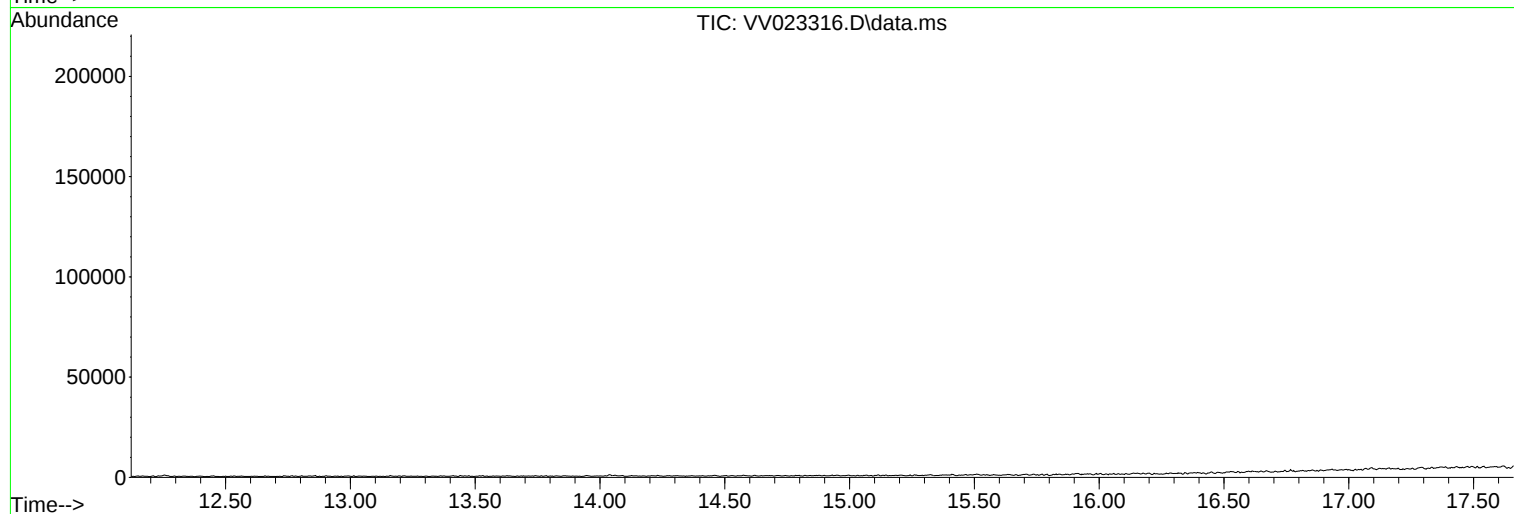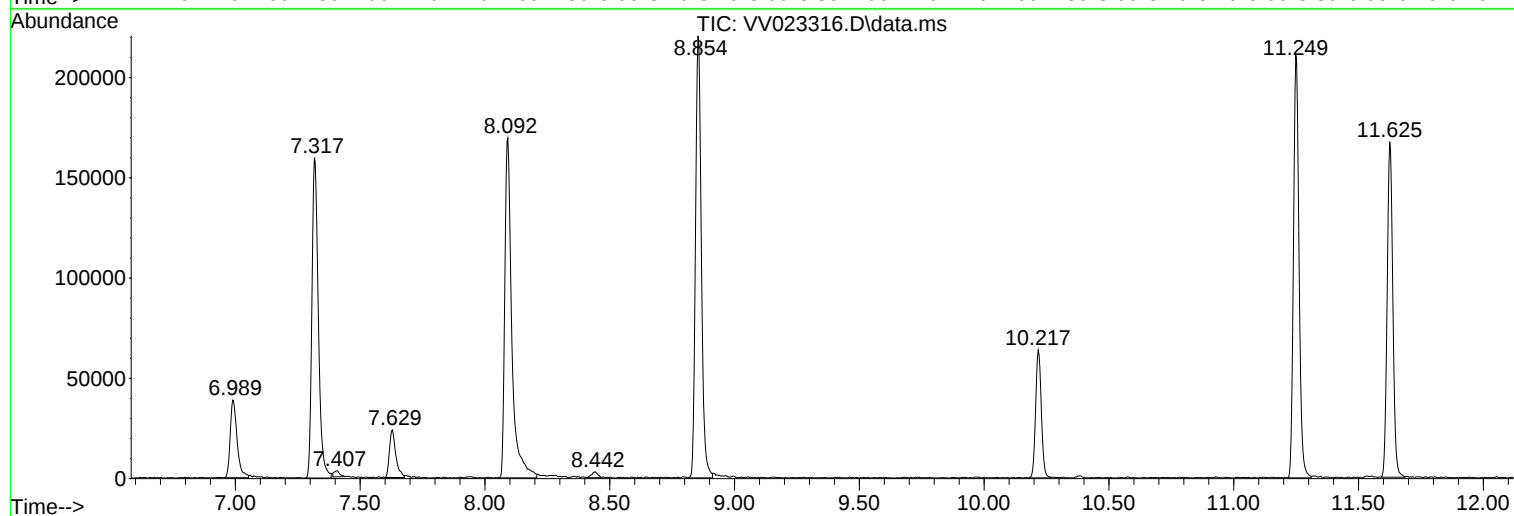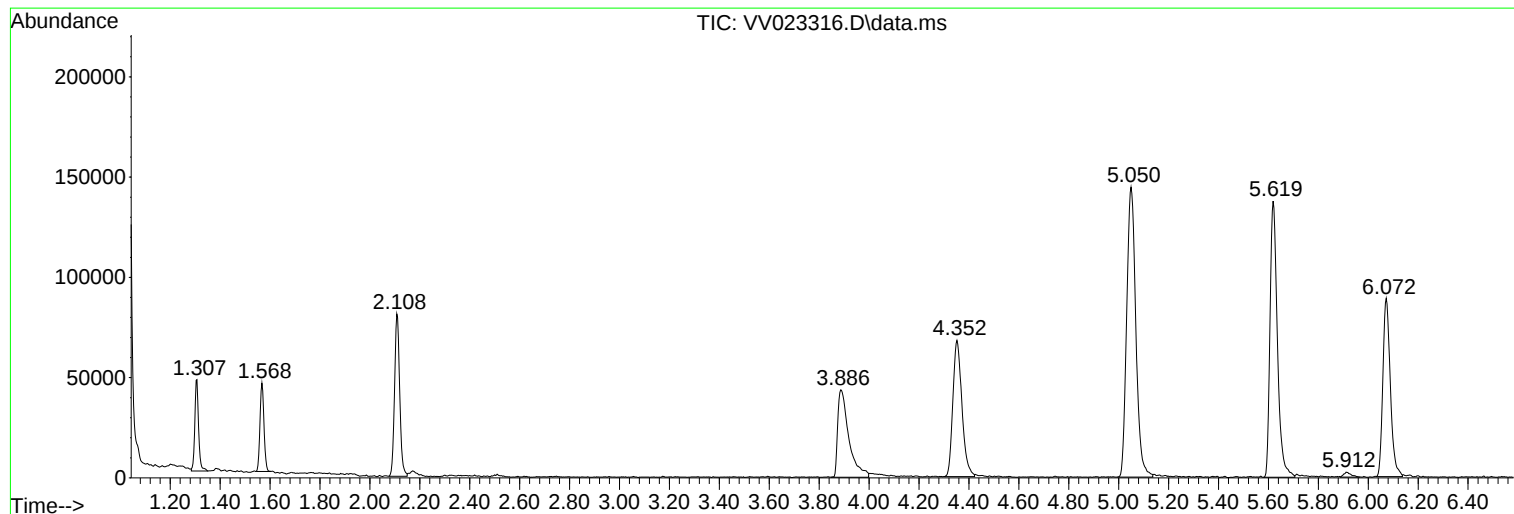

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023316.D
Acq On : 09 Nov 2021 20:17
Operator : SY/MD
Sample : M4522-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3A0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023316.D
Acq On : 09 Nov 2021 20:17
Operator : SY/MD
Sample : M4522-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3A0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc