

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
 Data File : VV023323.D
 Acq On : 10 Nov 2021 11:26
 Operator : SY/MD
 Sample : M4522-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3A7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023323.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	102	rVB	44246	47181	12.30%	1.388%
2	1.568	156	164	173	rBV	42549	48555	12.65%	1.429%
3	2.111	323	333	346	rBV	76040	111785	29.13%	3.289%
4	2.179	346	354	370	rVB	4194	9136	2.38%	0.269%
5	3.889	873	886	925	rBV	50089	156292	40.73%	4.598%
6	4.355	1013	1031	1055	rBV	73545	181097	47.20%	5.328%
7	5.050	1231	1247	1270	rBV3	150428	383683	100.00%	11.288%
8	5.619	1413	1424	1446	rBV	145210	298636	77.83%	8.786%
9	5.918	1515	1517	1528	rVB4	3801	4283	1.12%	0.126%
10	6.072	1550	1565	1588	rBV	94036	195931	51.07%	5.764%
11	6.992	1841	1851	1868	rBV	39453	73155	19.07%	2.152%
12	7.317	1941	1952	1970	rBV	166895	294595	76.78%	8.667%
13	7.400	1972	1978	1991	rVB	5400	9684	2.52%	0.285%
14	7.625	2038	2048	2072	rBV2	22665	44059	11.48%	1.296%
15	8.091	2183	2193	2227	rBV	182055	364902	95.11%	10.736%
16	8.854	2419	2430	2454	rBV	231988	380988	99.30%	11.209%
17	10.217	2843	2854	2869	rBV	65682	105266	27.44%	3.097%
18	11.249	3165	3175	3201	rBV	226076	352524	91.88%	10.371%
19	11.532	3254	3263	3277	rBV2	16787	29153	7.60%	0.858%
20	11.625	3280	3292	3311	rVB	186285	295911	77.12%	8.706%
21	12.001	3398	3409	3419	rBV7	3055	5016	1.31%	0.148%
22	12.345	3510	3516	3527	rVB5	4841	7151	1.86%	0.210%




Sum of corrected areas: 3398983

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023323.D
Acq On : 10 Nov 2021 11:26
Operator : SY/MD
Sample : M4522-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3A7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

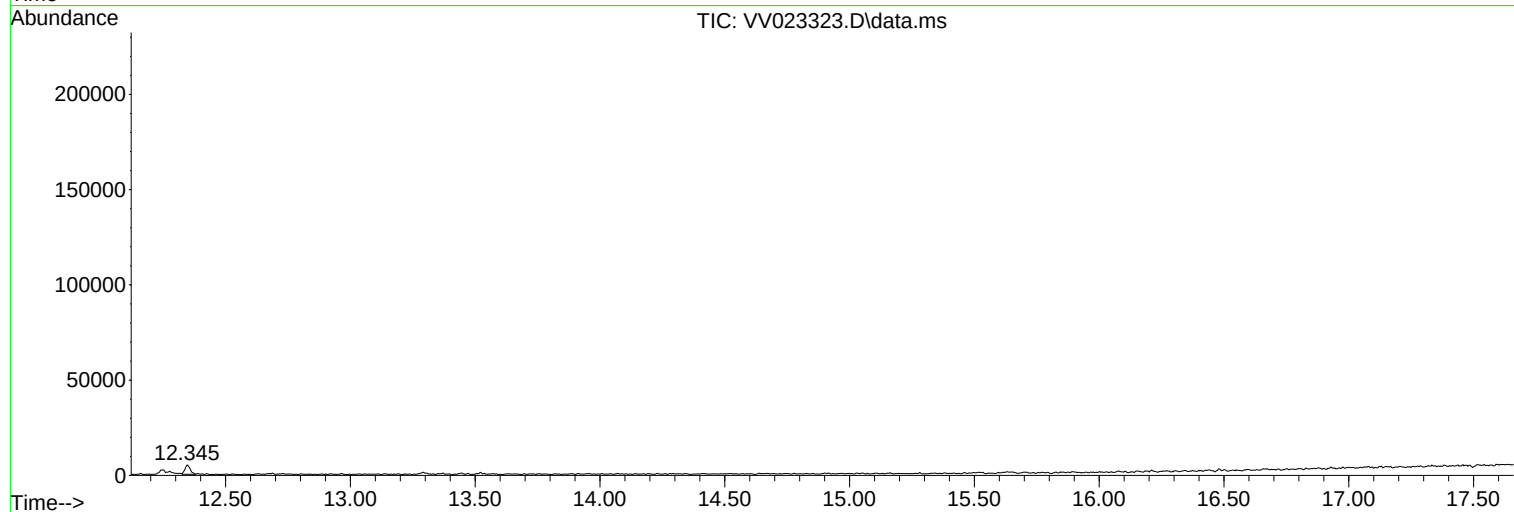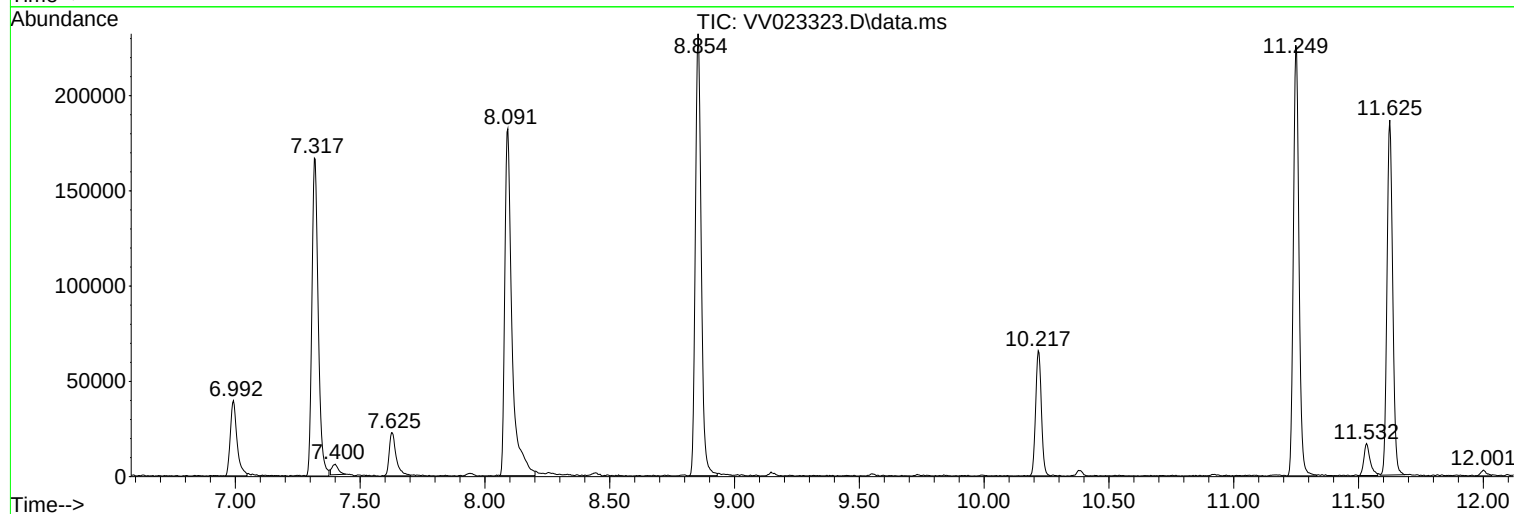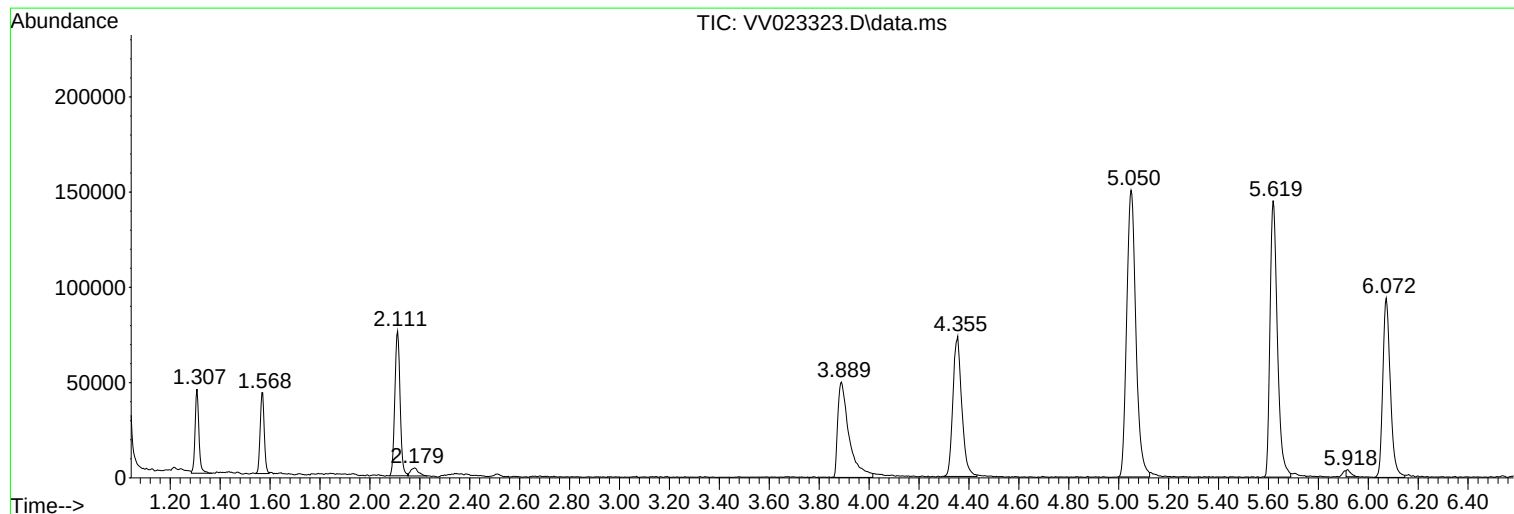

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023323.D
Acq On : 10 Nov 2021 11:26
Operator : SY/MD
Sample : M4522-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3A7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023323.D
Acq On : 10 Nov 2021 11:26
Operator : SY/MD
Sample : M4522-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3A7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
