

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
 Data File : VV023324.D
 Acq On : 10 Nov 2021 11:50
 Operator : SY/MD
 Sample : M4522-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023324.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	48858	49641	12.73%	1.494%
2	1.568	156	164	177	rBV	48751	55814	14.31%	1.680%
3	2.111	322	333	347	rBV	88693	127178	32.60%	3.828%
4	2.507	450	456	466	rVB4	2712	4192	1.07%	0.126%
5	3.889	876	886	915	rBV2	46896	141834	36.36%	4.269%
6	4.352	1014	1030	1055	rBV2	73340	186453	47.80%	5.612%
7	5.050	1231	1247	1270	rBV2	152060	390089	100.00%	11.741%
8	5.619	1413	1424	1453	rBV	142099	290255	74.41%	8.736%
9	5.915	1506	1516	1521	rBV6	2497	4067	1.04%	0.122%
10	6.072	1553	1565	1587	rBV2	94931	195444	50.10%	5.883%
11	6.989	1840	1850	1871	rBV	39745	74745	19.16%	2.250%
12	7.320	1939	1953	1972	rBV	169003	298984	76.65%	8.999%
13	7.625	2039	2048	2072	rBV3	24094	46146	11.83%	1.389%
14	8.091	2181	2193	2226	rBV	187226	360373	92.38%	10.847%
15	8.854	2416	2430	2456	rBV	223733	369641	94.76%	11.126%
16	10.217	2843	2854	2876	rBV2	68883	108961	27.93%	3.280%
17	10.381	2898	2905	2914	rVB3	2612	3987	1.02%	0.120%
18	11.249	3165	3175	3197	rBV	210343	333032	85.37%	10.024%
19	11.625	3280	3292	3309	rBV	177574	281576	72.18%	8.475%




Sum of corrected areas: 3322412

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023324.D
Acq On : 10 Nov 2021 11:50
Operator : SY/MD
Sample : M4522-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

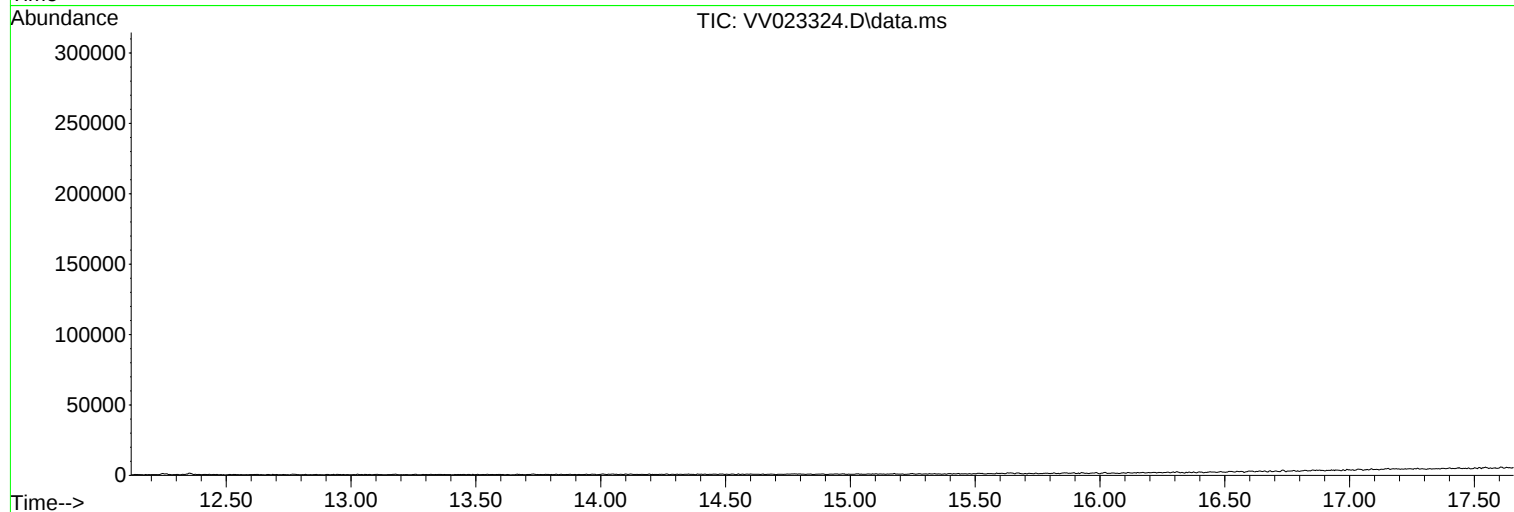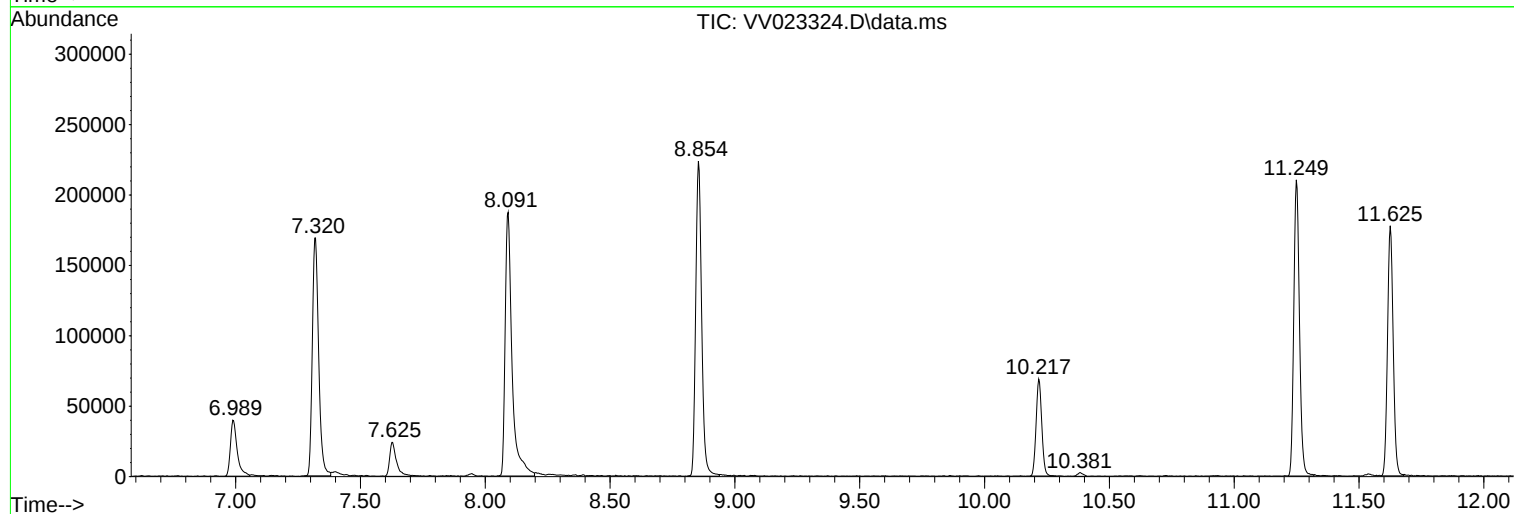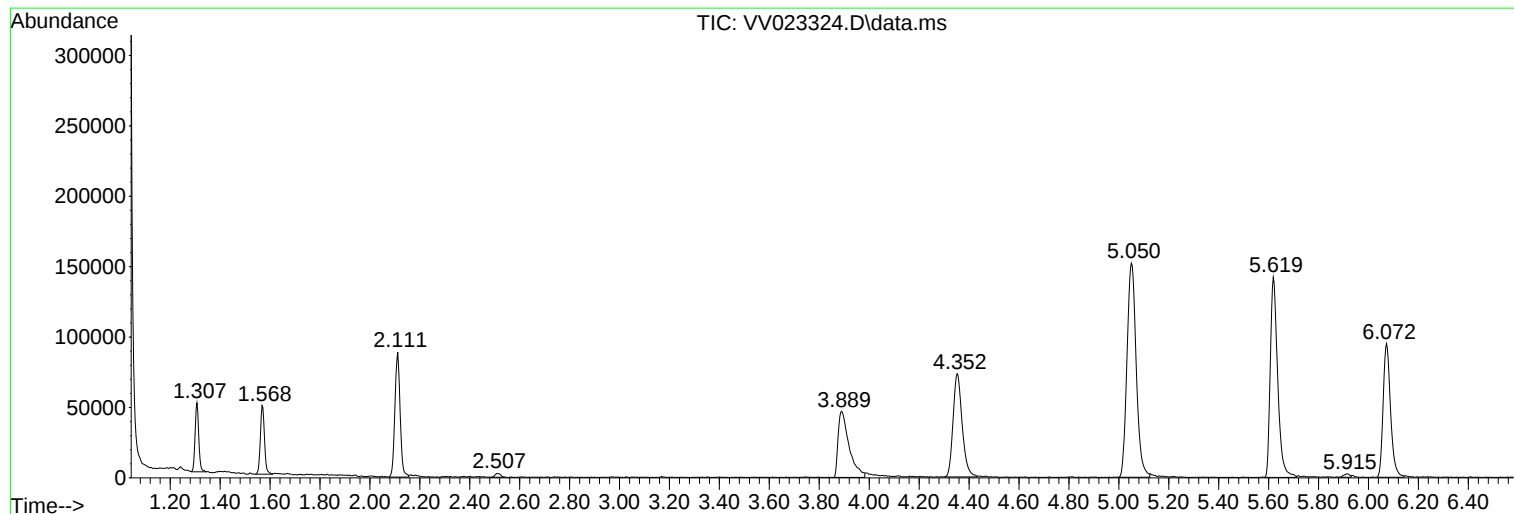

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023324.D
Acq On : 10 Nov 2021 11:50
Operator : SY/MD
Sample : M4522-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023324.D
Acq On : 10 Nov 2021 11:50
Operator : SY/MD
Sample : M4522-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
