

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
 Data File : VV023326.D
 Acq On : 10 Nov 2021 12:35
 Operator : SY/MD
 Sample : M4534-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023326.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	98	rVB	75403	76136	16.23%	2.104%
2	1.568	155	164	176	rBV	61937	71384	15.21%	1.973%
3	2.108	320	332	347	rBV	121067	173932	37.07%	4.807%
4	2.513	447	458	469	rBV	5420	9276	1.98%	0.256%
5	3.912	883	893	918	rBV	26289	102720	21.89%	2.839%
6	4.352	1013	1030	1057	rBV2	79457	203930	43.46%	5.636%
7	5.050	1230	1247	1286	rBV2	187212	469243	100.00%	12.969%
8	5.619	1413	1424	1446	rBV	134448	277339	59.10%	7.665%
9	5.915	1506	1516	1528	rBV9	3530	7234	1.54%	0.200%
10	6.072	1550	1565	1586	rBV2	105204	218384	46.54%	6.036%
11	6.989	1840	1850	1871	rBV	48671	93939	20.02%	2.596%
12	7.317	1941	1952	1971	rBV	216299	384507	81.94%	10.627%
13	7.625	2037	2048	2067	rBV2	28647	53228	11.34%	1.471%
14	8.095	2183	2194	2230	rBV	159613	347588	74.07%	9.606%
15	8.854	2414	2430	2447	rBV	216944	354566	75.56%	9.799%
16	10.217	2843	2854	2871	rBV	68342	111326	23.72%	3.077%
17	11.249	3165	3175	3191	rBV	214026	326653	69.61%	9.028%
18	11.625	3279	3292	3310	rBV	209965	331823	70.71%	9.171%
19	15.503	4492	4498	4508	rVB5	3534	5109	1.09%	0.141%




Sum of corrected areas: 3618317

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023326.D
Acq On : 10 Nov 2021 12:35
Operator : SY/MD
Sample : M4534-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

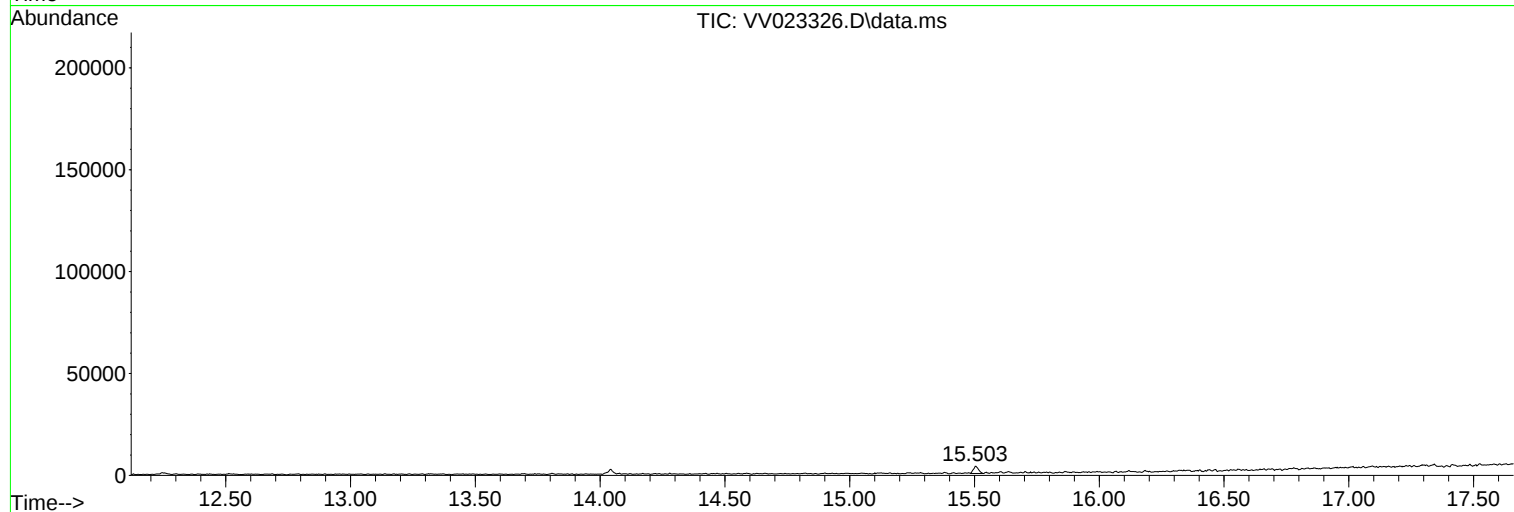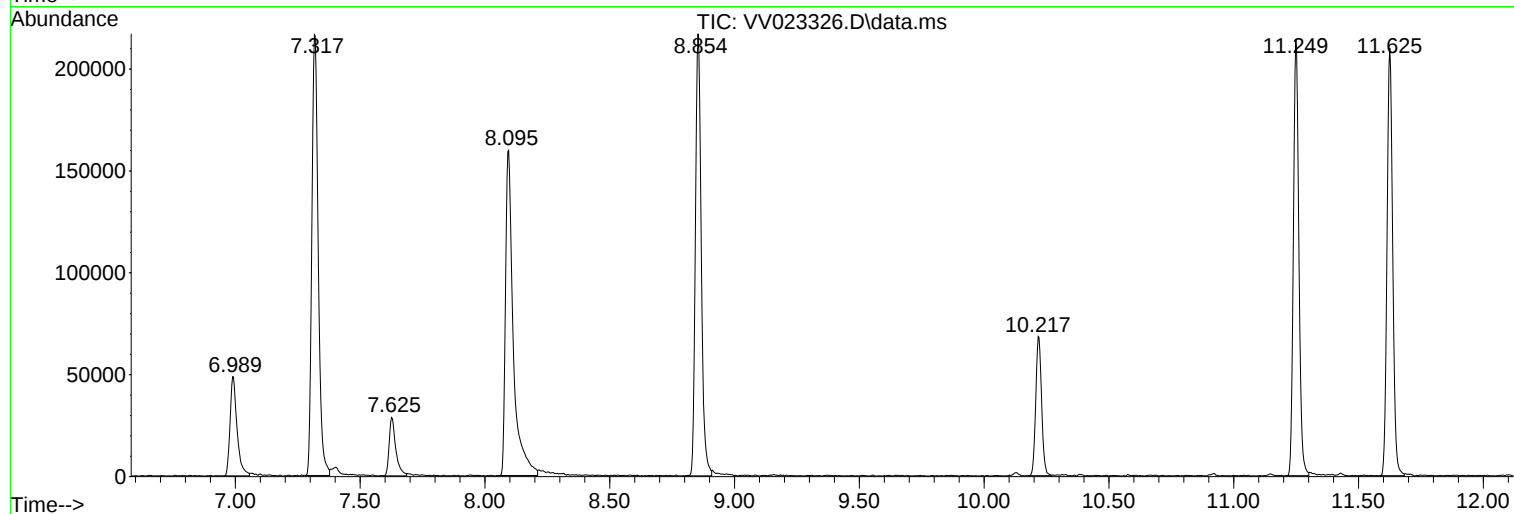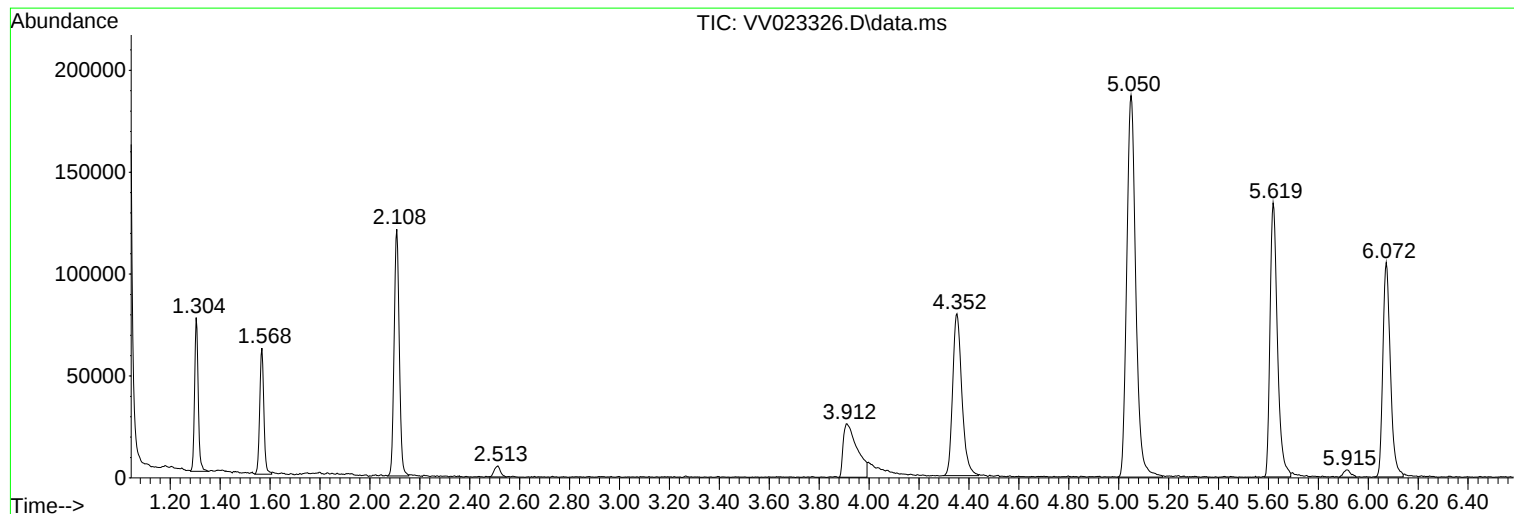

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023326.D
Acq On : 10 Nov 2021 12:35
Operator : SY/MD
Sample : M4534-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023326.D
Acq On : 10 Nov 2021 12:35
Operator : SY/MD
Sample : M4534-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
