

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
 Data File : VV023335.D
 Acq On : 10 Nov 2021 16:06
 Operator : SY/MD
 Sample : M4558-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB868

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023335.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	96	rVB	45377	48376	12.46%	1.463%
2	1.568	156	164	174	rBV	42689	49146	12.66%	1.487%
3	2.111	320	333	346	rBV	81154	118832	30.62%	3.594%
4	3.886	875	885	912	rBV2	50496	151950	39.15%	4.596%
5	4.352	1011	1030	1059	rBV3	78329	233868	60.26%	7.074%
6	5.050	1232	1247	1275	rBV2	152756	388127	100.00%	11.740%
7	5.619	1413	1424	1448	rBV	130745	269940	69.55%	8.165%
8	5.921	1506	1518	1534	rVB9	5450	12953	3.34%	0.392%
9	6.072	1552	1565	1595	rBV	92733	194255	50.05%	5.876%
10	6.516	1693	1703	1716	rBV	6539	12305	3.17%	0.372%
11	6.992	1839	1851	1870	rBV2	38387	72842	18.77%	2.203%
12	7.320	1942	1953	1969	rBV	168470	294647	75.92%	8.912%
13	7.625	2039	2048	2065	rBV2	23423	43286	11.15%	1.309%
14	7.982	2151	2159	2169	rVB6	3053	5159	1.33%	0.156%
15	8.091	2183	2193	2233	rBV	184421	364149	93.82%	11.015%
16	8.853	2418	2430	2454	rBV	207057	343353	88.46%	10.386%
17	10.217	2843	2854	2866	rBV	67269	107201	27.62%	3.243%
18	11.249	3164	3175	3191	rBV	199673	307006	79.10%	9.286%
19	11.532	3256	3263	3274	rBV5	2240	3954	1.02%	0.120%
20	11.625	3280	3292	3308	rBV	180255	284722	73.36%	8.612%




Sum of corrected areas: 3306071

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023335.D
Acq On : 10 Nov 2021 16:06
Operator : SY/MD
Sample : M4558-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB868

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

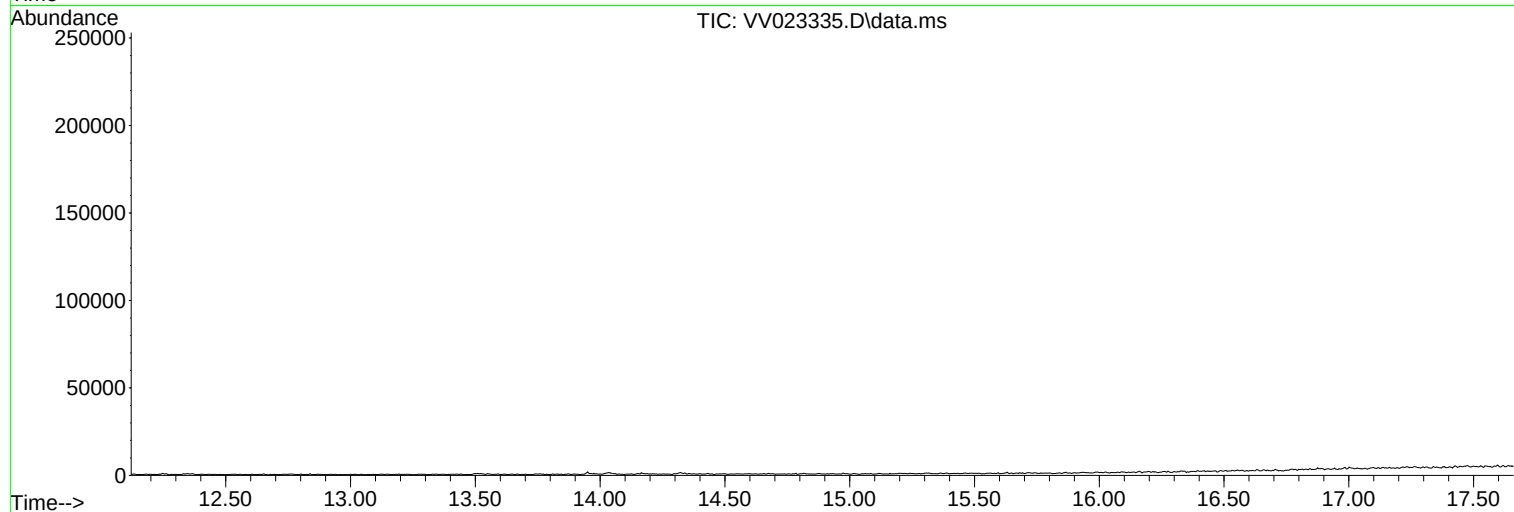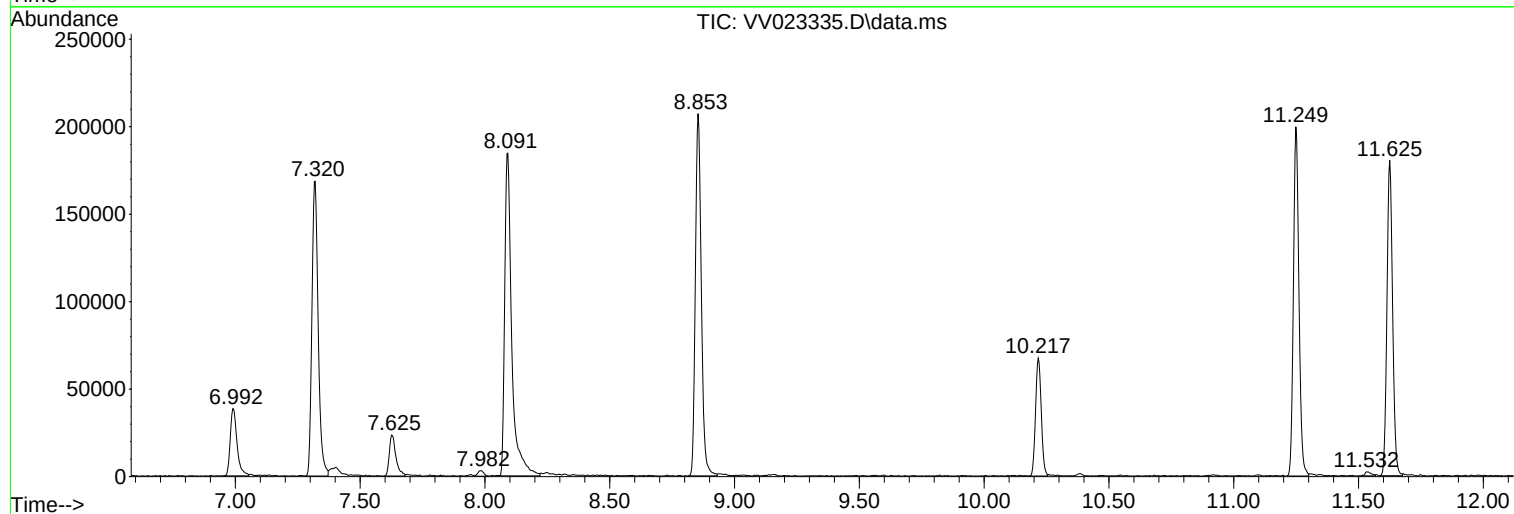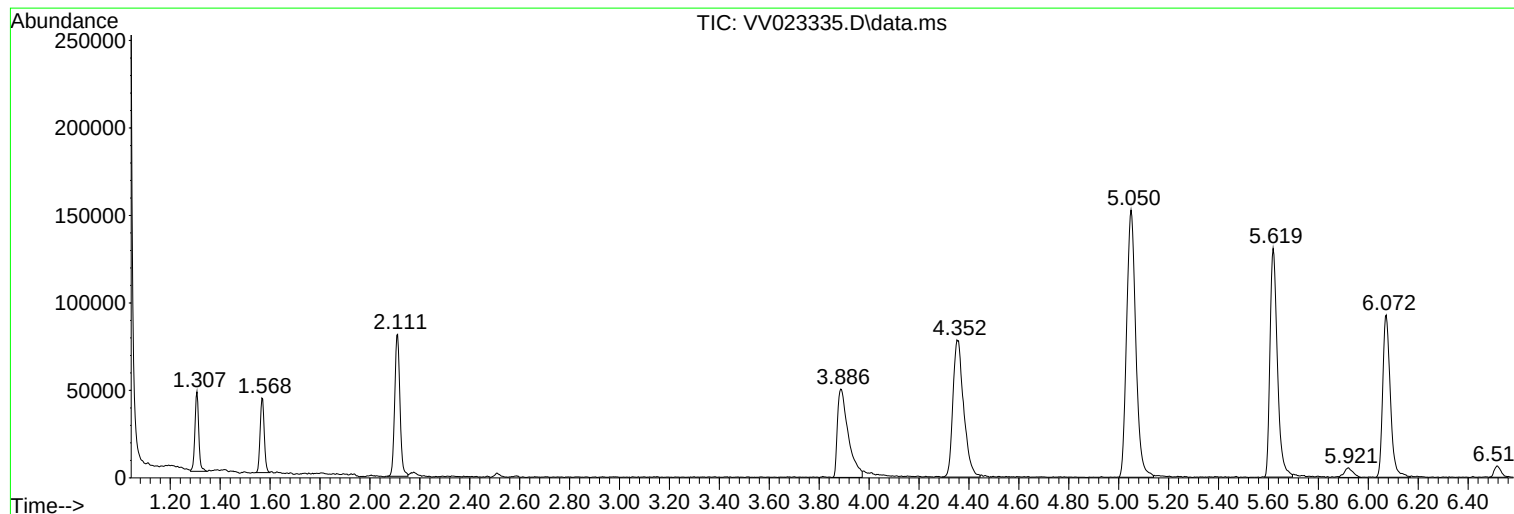

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023335.D
Acq On : 10 Nov 2021 16:06
Operator : SY/MD
Sample : M4558-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB868

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023335.D
Acq On : 10 Nov 2021 16:06
Operator : SY/MD
Sample : M4558-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB868

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc