

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
 Data File : VV023336.D
 Acq On : 10 Nov 2021 16:53
 Operator : SY/MD
 Sample : M4558-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB869

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023336.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rVB	43888	46881	12.01%	1.415%
2	1.568	156	164	175	rVB	43984	49902	12.78%	1.506%
3	2.108	323	332	347	rBV	78254	113213	29.01%	3.416%
4	3.905	881	891	923	rBV	36699	138389	35.46%	4.176%
5	4.355	1014	1031	1052	rBV3	71867	204537	52.40%	6.172%
6	5.050	1228	1247	1277	rBV2	155210	390322	100.00%	11.779%
7	5.619	1412	1424	1446	rBV	134285	276025	70.72%	8.329%
8	5.924	1504	1519	1537	rBV6	11381	27536	7.05%	0.831%
9	6.072	1550	1565	1591	rBV2	92307	195131	49.99%	5.888%
10	6.522	1695	1705	1715	rBV4	3545	6446	1.65%	0.195%
11	6.992	1841	1851	1869	rBV	37699	72675	18.62%	2.193%
12	7.320	1939	1953	1970	rBV	170690	300646	77.03%	9.072%
13	7.400	1972	1978	1990	rVB3	3733	7261	1.86%	0.219%
14	7.628	2040	2049	2062	rBV2	22474	42116	10.79%	1.271%
15	7.982	2151	2159	2167	rBV3	3399	5130	1.31%	0.155%
16	8.091	2182	2193	2228	rBV	183831	372646	95.47%	11.245%
17	8.853	2419	2430	2450	rBV	214120	350096	89.69%	10.565%
18	10.217	2844	2854	2870	rBV	67983	108290	27.74%	3.268%
19	11.249	3165	3175	3192	rBV	198819	317098	81.24%	9.569%
20	11.625	3281	3292	3307	rBV	183658	289494	74.17%	8.736%




Sum of corrected areas: 3313834

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023336.D
Acq On : 10 Nov 2021 16:53
Operator : SY/MD
Sample : M4558-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB869

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

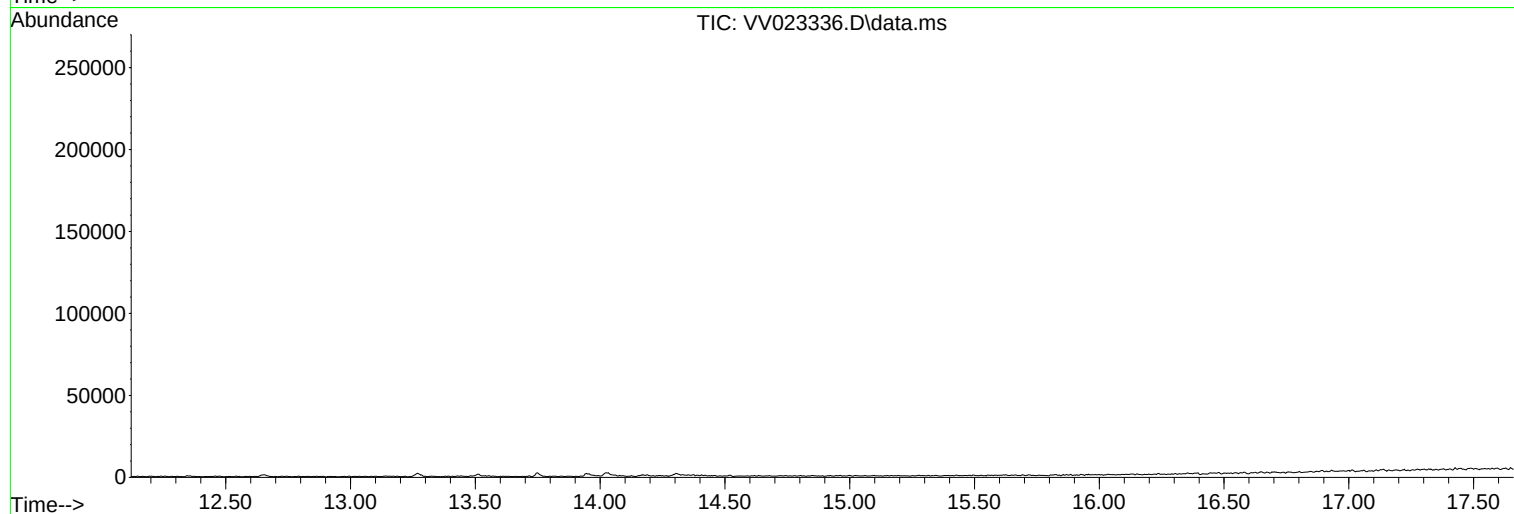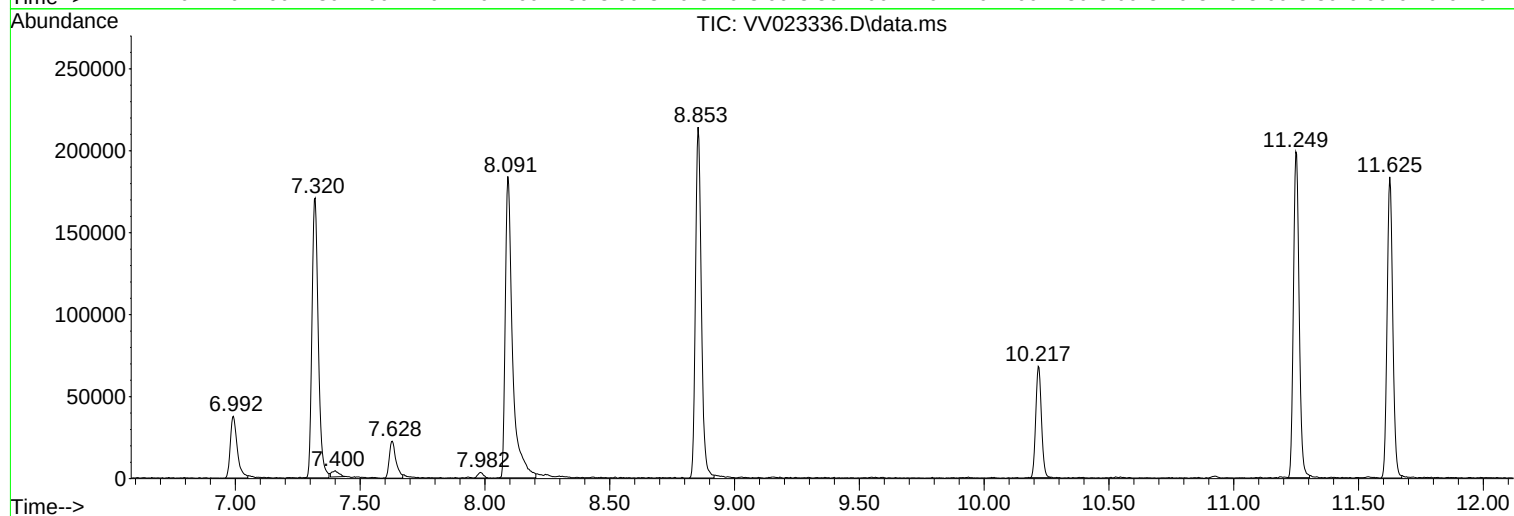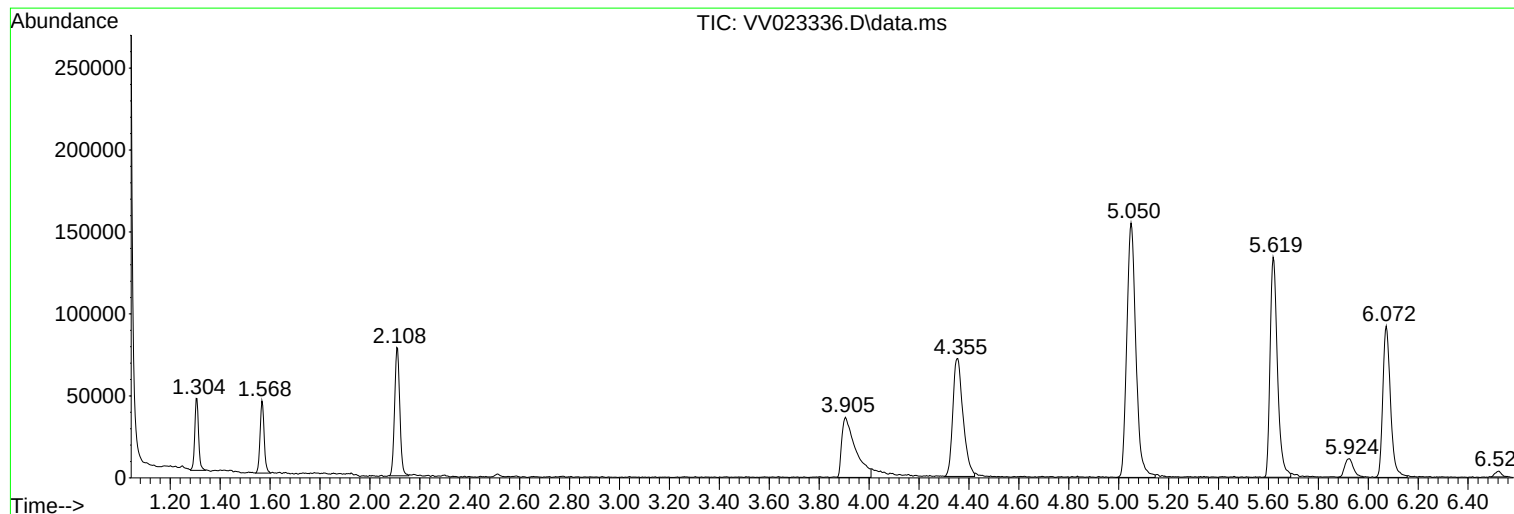

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023336.D
Acq On : 10 Nov 2021 16:53
Operator : SY/MD
Sample : M4558-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB869

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023336.D
Acq On : 10 Nov 2021 16:53
Operator : SY/MD
Sample : M4558-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB869

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc