

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
 Data File : VV023341.D
 Acq On : 10 Nov 2021 18:50
 Operator : SY/MD
 Sample : M4535-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4565

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023341.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	96	rVB	75402	75201	16.09%	1.777%
2	1.568	155	164	177	rBV	53082	59687	12.77%	1.410%
3	1.635	177	185	195	rVB2	10293	13917	2.98%	0.329%
4	2.108	322	332	346	rBV	105741	156196	33.41%	3.690%
5	2.182	346	355	373	rVB3	5566	12586	2.69%	0.297%
6	2.297	378	391	405	rBV	285026	422467	90.37%	9.980%
7	2.513	442	458	472	rBV	3208	8292	1.77%	0.196%
8	3.892	876	887	920	rBV2	43973	136249	29.14%	3.219%
9	4.352	1014	1030	1056	rBV2	73589	186761	39.95%	4.412%
10	5.050	1232	1247	1284	rBV2	173353	467503	100.00%	11.044%
11	5.619	1412	1424	1447	rBV	172361	348909	74.63%	8.242%
12	5.915	1506	1516	1527	rVB7	3775	7325	1.57%	0.173%
13	6.072	1553	1565	1590	rBV	96595	200976	42.99%	4.748%
14	6.992	1840	1851	1868	rBV2	45988	86614	18.53%	2.046%
15	7.320	1941	1953	1971	rBV	212839	373834	79.96%	8.831%
16	7.400	1972	1978	1987	rVB5	4130	7042	1.51%	0.166%
17	7.628	2036	2049	2069	rBV2	26674	50695	10.84%	1.198%
18	8.091	2183	2193	2225	rBV	163682	316107	67.62%	7.468%
19	8.853	2419	2430	2452	rBV	262741	430346	92.05%	10.166%
20	10.217	2843	2854	2867	rBV	60827	94167	20.14%	2.225%
21	10.387	2897	2907	2915	rVB4	3225	4881	1.04%	0.115%
22	11.249	3163	3175	3198	rBV	269277	416009	88.99%	9.828%
23	11.625	3280	3292	3313	rBV	196110	315772	67.54%	7.460%
24	12.252	3477	3487	3495	rVB2	4732	6889	1.47%	0.163%
25	12.352	3508	3518	3531	rBV5	7003	11272	2.41%	0.266%
26	14.040	4032	4043	4057	rBV2	12940	23374	5.00%	0.552%




Sum of corrected areas: 4233071

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023341.D
Acq On : 10 Nov 2021 18:50
Operator : SY/MD
Sample : M4535-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4565

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

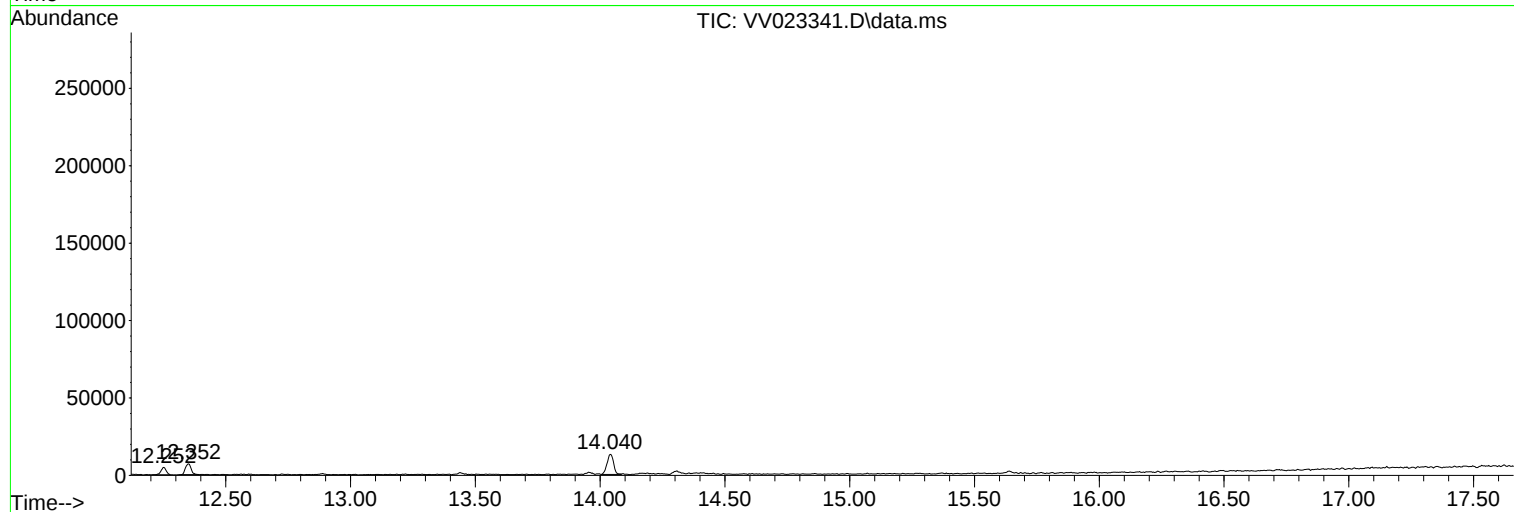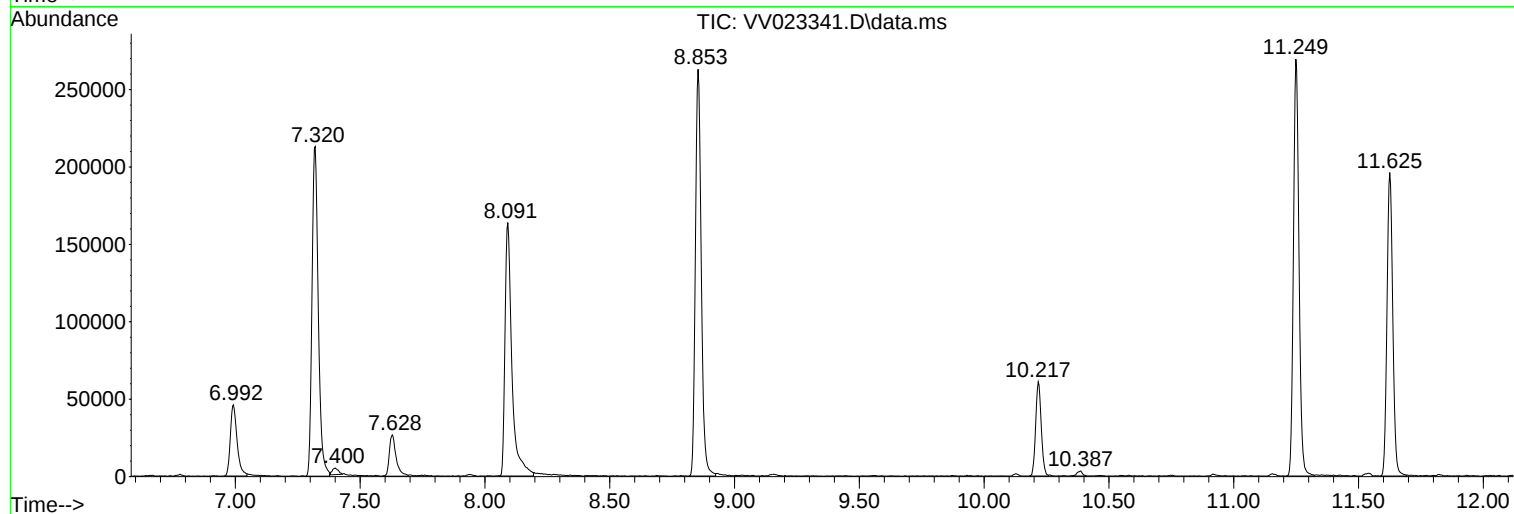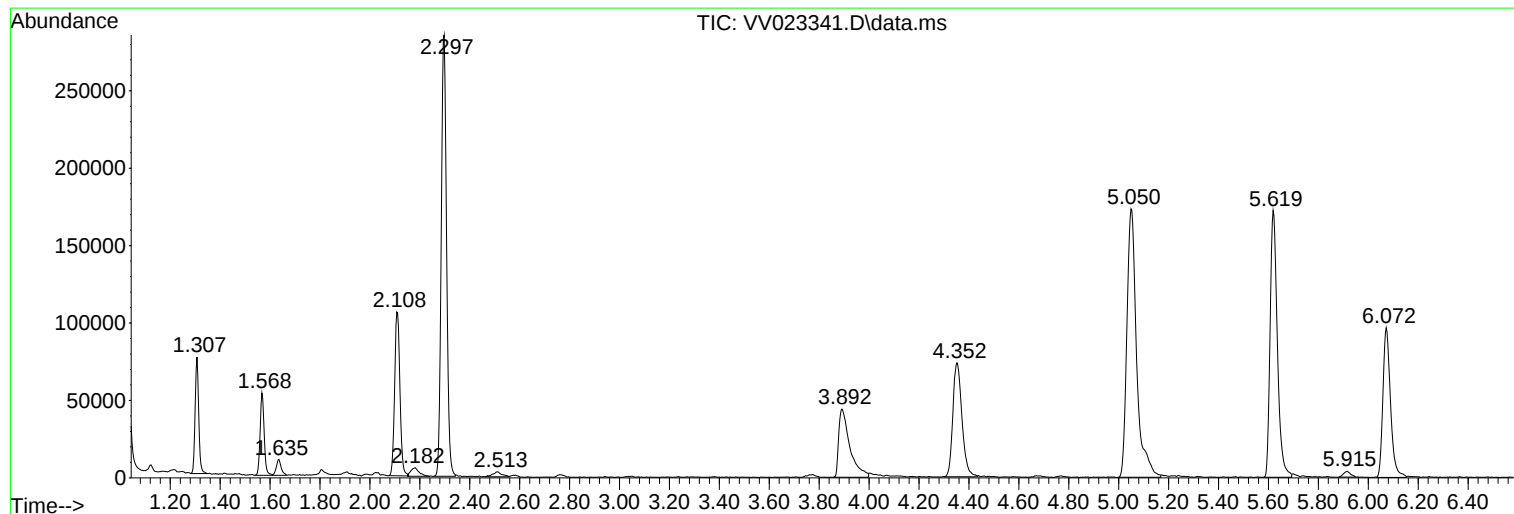

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023341.D
Acq On : 10 Nov 2021 18:50
Operator : SY/MD
Sample : M4535-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4565

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023341.D
Acq On : 10 Nov 2021 18:50
Operator : SY/MD
Sample : M4535-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4565

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc