

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
 Data File : VV023343.D
 Acq On : 10 Nov 2021 19:37
 Operator : SY/MD
 Sample : M4535-22
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4566

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023343.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	95	rVB	65316	66409	15.45%	1.835%
2	1.568	155	164	175	rBV	47666	55477	12.90%	1.533%
3	1.632	178	184	191	rVB4	5100	6115	1.42%	0.169%
4	2.108	321	332	344	rBV	102171	148580	34.56%	4.106%
5	2.179	347	354	362	rVB2	3826	6990	1.63%	0.193%
6	2.298	381	391	402	rVB	2916	4854	1.13%	0.134%
7	2.510	443	457	466	rBV9	2438	5495	1.28%	0.152%
8	3.892	877	887	926	rBV	44585	138718	32.27%	3.833%
9	4.352	1014	1030	1053	rBV2	69132	177332	41.25%	4.901%
10	5.050	1230	1247	1280	rBV3	166773	429903	100.00%	11.880%
11	5.619	1411	1424	1452	rBV	164692	332480	77.34%	9.188%
12	6.072	1551	1565	1584	rBV2	93480	191920	44.64%	5.304%
13	6.989	1839	1850	1872	rBV	43289	83368	19.39%	2.304%
14	7.317	1940	1952	1970	rBV	195503	345208	80.30%	9.540%
15	7.629	2039	2049	2065	rBV	26680	48215	11.22%	1.332%
16	8.092	2183	2193	2234	rBV	170103	337269	78.45%	9.320%
17	8.854	2419	2430	2451	rBV	244937	405056	94.22%	11.194%
18	10.217	2843	2854	2867	rBV2	60493	96438	22.43%	2.665%
19	10.384	2894	2906	2919	rVB3	6737	11684	2.72%	0.323%
20	11.249	3164	3175	3189	rBV	255676	392017	91.19%	10.833%
21	11.625	3281	3292	3310	rBV	192755	301202	70.06%	8.324%
22	12.249	3477	3486	3498	rVB	6659	10199	2.37%	0.282%
23	14.040	4034	4043	4059	rVB2	13370	23682	5.51%	0.654%




Sum of corrected areas: 3618611

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023343.D
Acq On : 10 Nov 2021 19:37
Operator : SY/MD
Sample : M4535-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4566

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

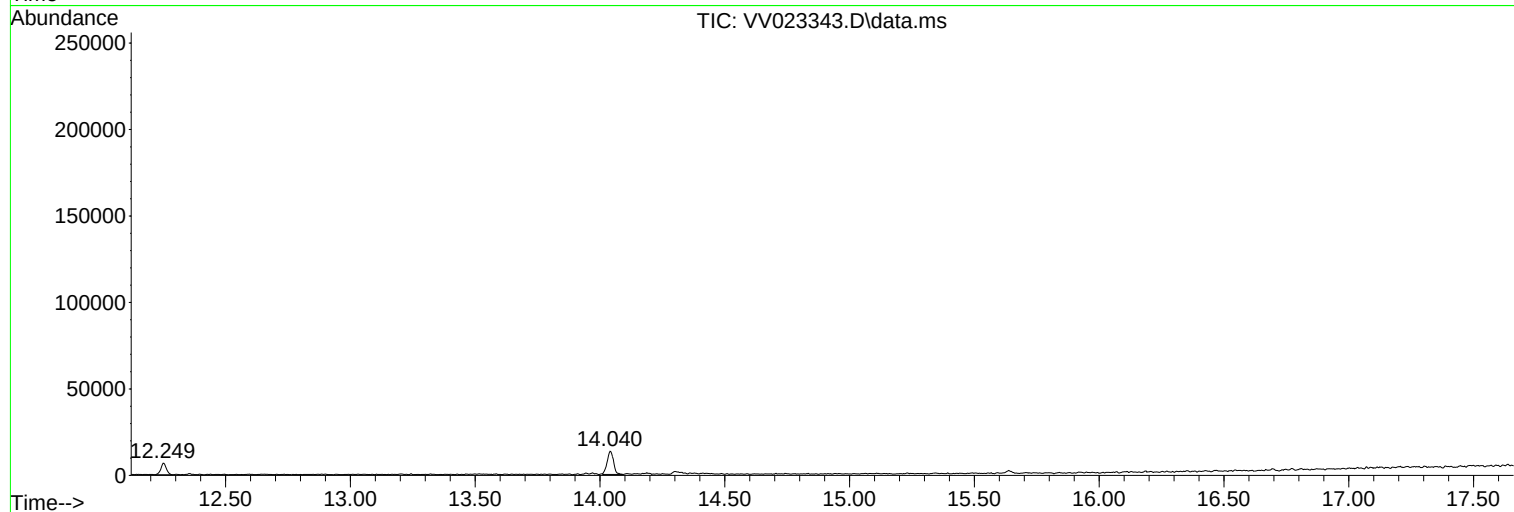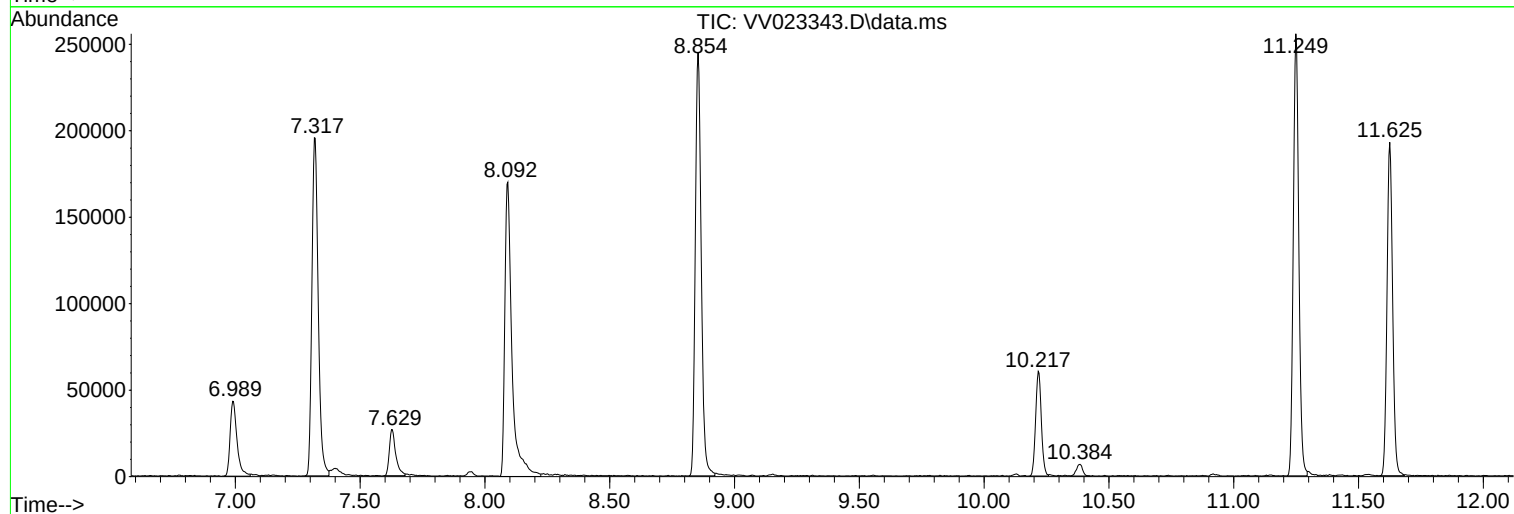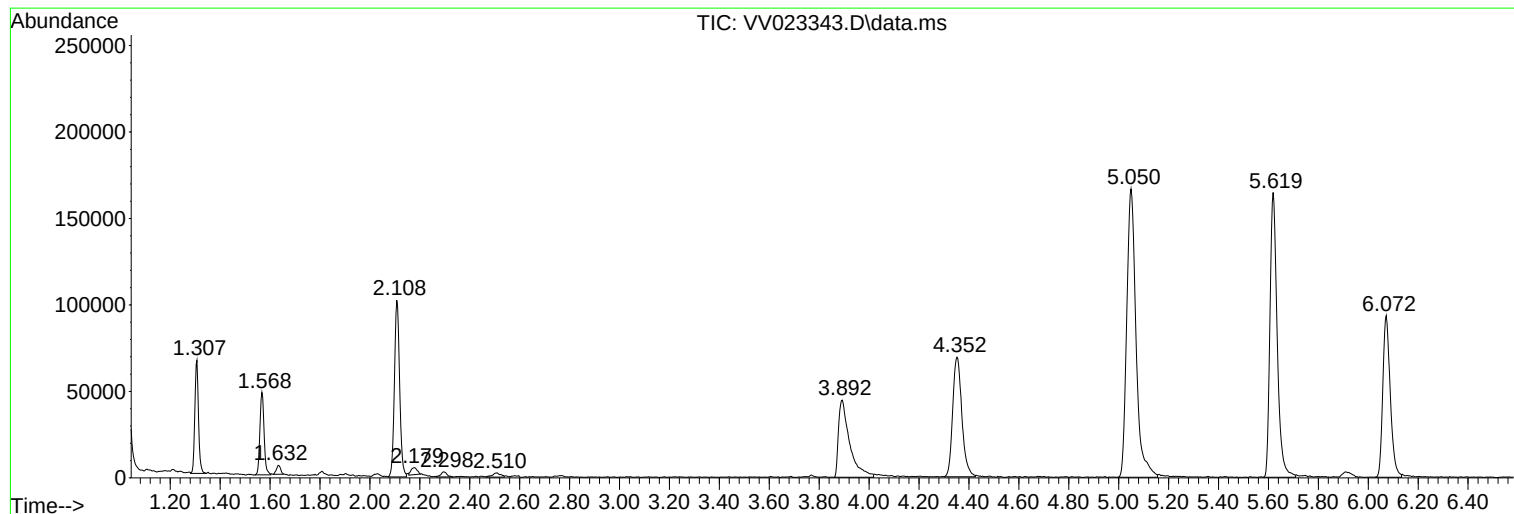

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023343.D
Acq On : 10 Nov 2021 19:37
Operator : SY/MD
Sample : M4535-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4566

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
Data File : VV023343.D
Acq On : 10 Nov 2021 19:37
Operator : SY/MD
Sample : M4535-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4566

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc