
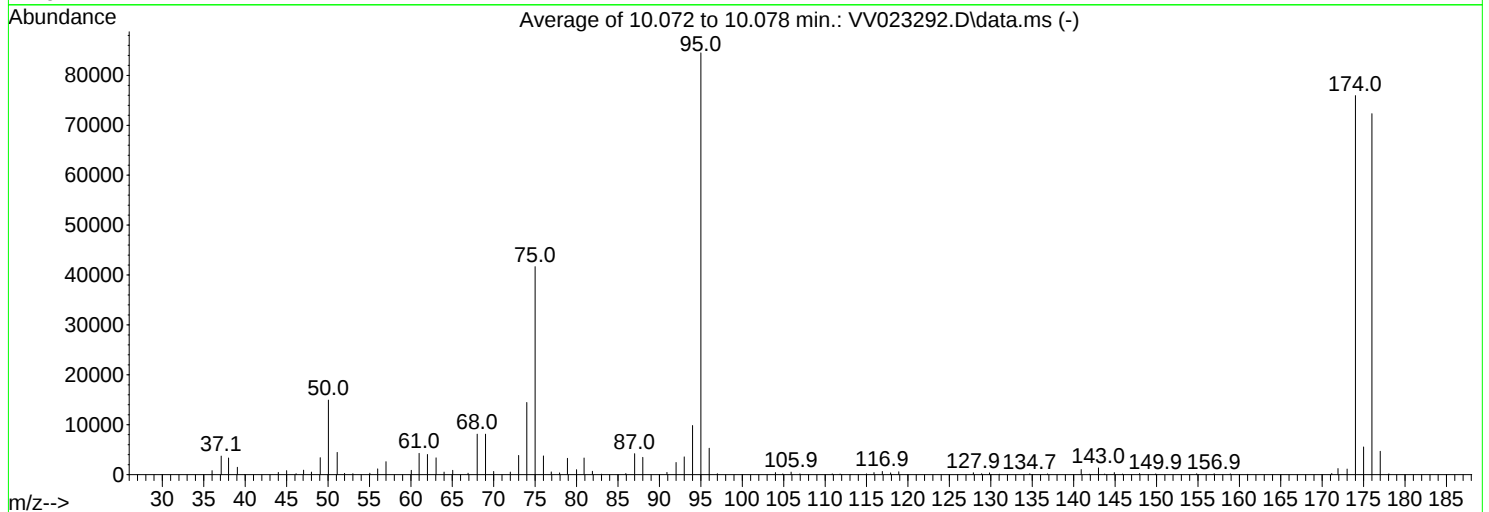


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110921\
 Data File : VV023292.D
 Acq On : 09 Nov 2021 09:58
 Operator : SY/MD
 Sample : BFB230
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB230

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Nov 17 00:48:57 2021

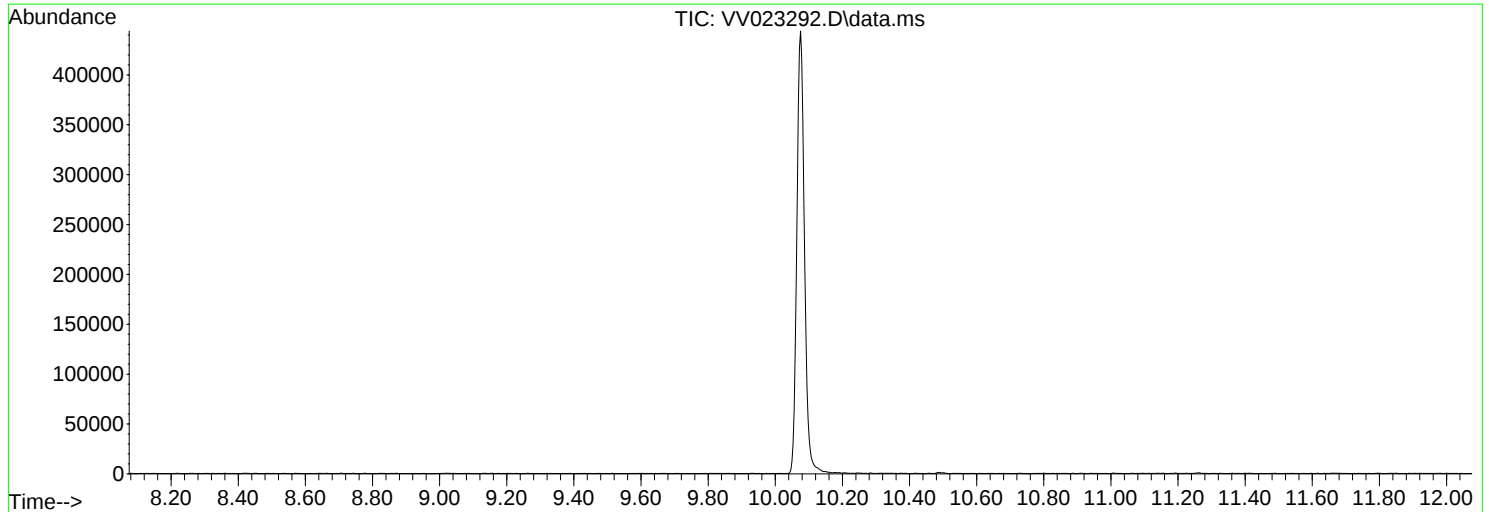

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	14950	PASS
75	95	30	80	49.3	41693	PASS
95	95	100	100	100.0	84515	PASS
96	95	5	9	6.3	5292	PASS
173	174	0.00	2	1.5	1110	PASS
174	95	50	120	89.8	75936	PASS
175	174	5	9	7.3	5547	PASS
176	174	95	105	95.3	72336	PASS
177	176	5	10	6.5	4672	PASS

m/z	Abundance
36.30	112.0
40.00	142.0
44.00	224.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

m/z	Abundance
36.00	853.0
37.10	3785.0
38.00	3401.0
39.00	1383.0
39.80	146.0
44.00	646.0
45.00	808.0
46.20	185.0
47.10	793.0
48.00	515.0
49.00	3428.0
50.10	15042.0
51.10	4508.0
52.00	239.0
53.00	227.0
55.10	288.0
56.00	1159.0
57.00	2471.0
60.00	795.0
61.00	4317.0
62.00	4131.0
63.10	3319.0
64.00	476.0
65.10	822.0
66.90	274.0
68.00	8230.0
69.00	8247.0
70.00	685.0
72.00	478.0
73.00	3787.0
74.00	14198.0
75.00	41640.0
76.00	3844.0
76.90	514.0
77.90	364.0
78.90	3350.0
80.00	986.0
80.90	3316.0
81.90	686.0
83.00	156.0
85.90	202.0
87.00	4404.0
88.00	3631.0
90.90	444.0
92.00	2543.0
93.00	3493.0
94.00	9889.0
95.00	84376.0
96.00	5519.0
97.00	219.0
104.00	412.0
104.90	178.0
105.90	565.0
106.90	141.0
110.90	166.0
111.80	115.0
115.00	130.0
115.80	395.0
116.90	748.0
117.90	323.0
118.90	568.0
127.90	428.0
128.90	243.0
129.90	311.0
131.00	107.0
134.70	187.0
136.90	135.0
140.90	1009.0
141.90	179.0
143.00	1488.0
143.80	107.0
144.90	418.0
145.90	120.0
148.00	215.0
149.90	160.0
154.80	156.0
157.00	186.0
158.90	168.0
161.00	144.0
171.10	186.0
171.90	1150.0
173.00	1063.0
174.00	73856.0
175.00	5429.0
176.00	71176.0
177.00	4600.0
178.10	173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

m/z	Abundance
36.00	844.0
37.10	3868.0
38.00	3432.0
39.00	1526.0
39.90	169.0
44.00	672.0
45.00	817.0
46.10	208.0
47.00	915.0
48.00	542.0
49.10	3546.0
50.10	15549.0
51.10	4607.0
52.00	267.0
53.00	221.0
55.00	305.0
56.00	1168.0
57.00	2699.0
60.00	887.0
61.00	4486.0
62.00	4162.0
63.10	3447.0
64.00	499.0
65.00	900.0
66.90	309.0
68.00	8374.0
69.00	8404.0
70.00	664.0
72.00	549.0
73.00	3991.0
74.00	15090.0
75.00	43088.0
76.00	3923.0
77.00	514.0
77.90	364.0
78.90	3334.0
80.00	1043.0
80.90	3429.0
81.90	655.0
83.00	113.0
85.90	225.0
87.00	4408.0
88.00	3589.0
90.90	460.0
92.00	2489.0
93.00	3701.0
94.00	10128.0
95.00	87432.0
96.00	5435.0
97.00	198.0
104.00	438.0
104.90	167.0
105.90	527.0
107.00	193.0
110.80	157.0
111.80	131.0
115.00	176.0
115.90	417.0
116.90	670.0
117.90	368.0
118.90	579.0
127.90	412.0
128.90	201.0
129.80	340.0
131.10	101.0
134.70	217.0
136.90	147.0
140.90	1063.0
141.90	135.0
143.00	1394.0
143.70	153.0
144.90	440.0
145.90	131.0
147.90	226.0
149.90	169.0
154.90	217.0
156.90	221.0
158.90	161.0
161.00	101.0
171.20	229.0
171.90	1265.0
173.00	1138.0
174.00	78552.0
175.00	5759.0
176.00	74800.0
177.00	4845.0
178.10	180.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230

m/z	Abundance
36.00	745.0
37.10	3511.0
38.00	3196.0
39.10	1564.0
40.00	190.0
44.00	662.0
45.00	739.0
46.10	200.0
47.00	1024.0
48.00	513.0
49.10	3240.0
50.00	14259.0
51.10	4236.0
52.00	276.0
53.00	186.0
55.00	271.0
56.00	1157.0
57.00	2601.0
60.10	905.0
61.00	4042.0
62.00	3832.0
63.00	3305.0
64.00	530.0
65.00	846.0
66.90	307.0
68.00	7699.0
69.00	7691.0
70.00	606.0
72.00	548.0
73.00	3774.0
74.00	14048.0
75.00	40352.0
76.00	3532.0
77.00	583.0
78.00	323.0
78.90	3178.0
80.00	964.0
80.90	3300.0
81.90	659.0
86.00	228.0
87.00	3788.0
88.00	3144.0
90.90	410.0
92.00	2295.0
93.00	3455.0
94.00	9477.0
95.00	81736.0
96.00	4923.0
97.00	168.0
104.00	404.0
104.90	150.0
105.90	419.0
107.00	201.0
110.80	125.0
111.80	112.0
113.10	106.0
115.00	157.0
116.00	419.0
116.90	538.0
117.90	382.0
118.90	570.0
127.90	358.0
128.90	182.0
129.90	373.0
131.10	108.0
134.70	212.0
136.80	173.0
140.90	999.0
143.00	1201.0
143.70	147.0
144.90	421.0
145.90	131.0
147.90	258.0
149.90	152.0
153.00	110.0
154.90	225.0
156.90	217.0
158.90	130.0
171.20	250.0
171.90	1236.0
173.00	1130.0
174.00	75400.0
175.00	5454.0
176.00	71032.0
177.00	4570.0
178.00	164.0

Instrument :
MSVOA_V
ClientSampleId :
BFB230