

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110922\
 Data File : VV028854.D
 Acq On : 09 Nov 2022 10:00
 Operator : SY/MD
 Sample : VV1109MBL01
 Misc : 5.00g/5.00mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK288

Quant Time: Nov 10 00:44:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Nov 10 00:43:48 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.606	114	392514	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	356670	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	159906	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	169472	45.546	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	91.100%		
7) Chloroethane-d5	1.561	69	145794	45.835	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	91.660%		
11) 1,1-Dichloroethene-d2	2.101	63	244114	34.489	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	68.980%		
21) 2-Butanone-d5	3.863	46	206796	76.348	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	76.350%		
24) Chloroform-d	4.333	84	254436	45.338	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.680%		
26) 1,2-Dichloroethane-d4	5.021	65	172732	46.539	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.080%		
32) Benzene-d6	5.040	84	529753	47.578	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.160%		
36) 1,2-Dichloropropane-d6	6.059	67	181473	47.474	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	94.940%		
41) Toluene-d8	7.307	98	451096	46.085	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.160%		
43) trans-1,3-Dichloroprop...	7.612	79	69581	47.393	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	94.780%		
47) 2-Hexanone-d5	8.082	63	124192	71.892	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	71.890%		
56) 1,1,2,2-Tetrachloroeth...	10.207	84	208817	41.426	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	82.860%		
66) 1,2-Dichlorobenzene-d4	11.615	152	147768	46.815	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.640%		
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.104	101	2039	0.686	ug/L	# 27


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110922\
Data File : VV028854.D
Acq On : 09 Nov 2022 10:00
Operator : SY/MD
Sample : VV1109MBL01
Misc : 5.00g/5.00mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK288

Quant Time: Nov 10 00:44:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Nov 10 00:43:48 2022
Response via : Initial Calibration

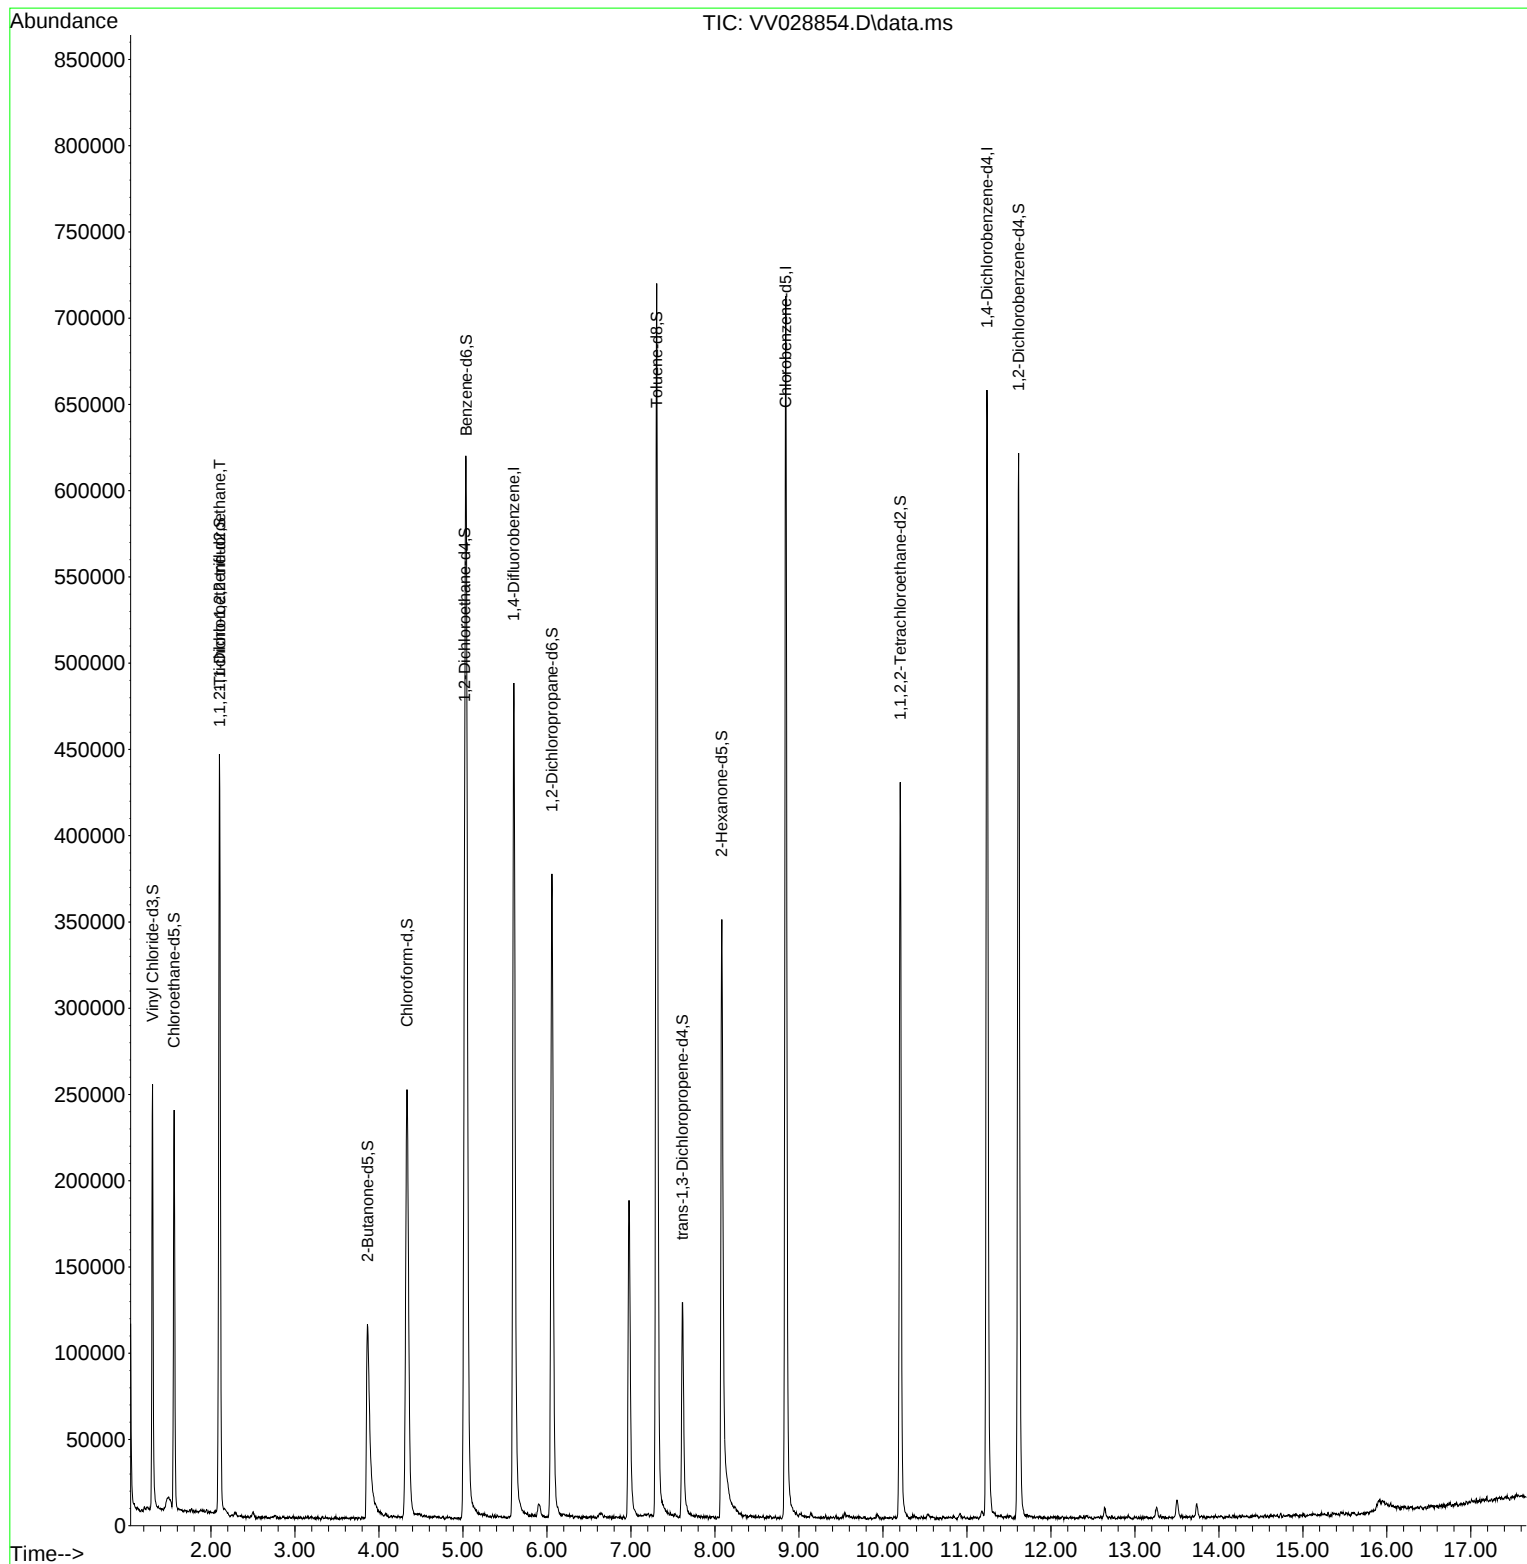

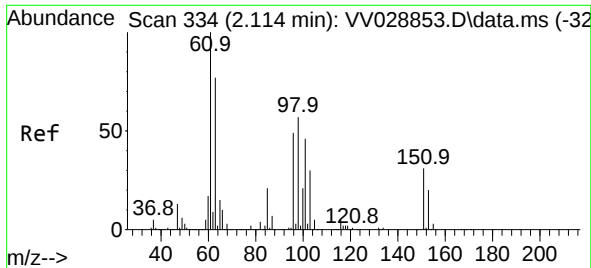

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.686 ug/L
 RT: 2.104 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV028854.D
 Acq: 09 Nov 2022 10:00

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK288

Tgt Ion:101 Resp: 2039
 Ion Ratio Lower Upper
 101 100
 85 4.7 38.0 57.0#
 151 2.0 52.7 79.1#

