

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW110922\
 Data File : VW028856.D
 Acq On : 09 Nov 2022 11:09
 Operator : SY/MD
 Sample : N5519-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C1122

Quant Time: Nov 10 00:44:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Nov 10 00:43:48 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.606	114	381281	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	349740	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	157356	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	182766	50.565	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	101.140%
7) Chloroethane-d5	1.565	69	158396	51.264	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	102.520%
11) 1,1-Dichloroethene-d2	2.105	63	269378	39.179	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.360%
21) 2-Butanone-d5	3.867	46	209225	79.520	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	79.520%
24) Chloroform-d	4.336	84	278533	51.094	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.180%
26) 1,2-Dichloroethane-d4	5.021	65	189459	52.550	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.100%
32) Benzene-d6	5.040	84	583090	53.406	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.820%
36) 1,2-Dichloropropane-d6	6.060	67	200374	53.457	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	106.920%
41) Toluene-d8	7.307	98	504606	52.573	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.140%
43) trans-1,3-Dichloroprop...	7.613	79	76813	53.356	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	106.720%
47) 2-Hexanone-d5	8.082	63	124001	73.204	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	73.200%
56) 1,1,2,2-Tetrachloroeth...	10.207	84	227950	46.118	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.240%
66) 1,2-Dichlorobenzene-d4	11.616	152	164345	52.911	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.820%
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.105	101	2324	0.805	ug/L	# 24
13) Acetone	2.159	43	18114	7.111	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110922\
Data File : VV028856.D
Acq On : 09 Nov 2022 11:09
Operator : SY/MD
Sample : N5519-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C1122

Quant Time: Nov 10 00:44:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Nov 10 00:43:48 2022
Response via : Initial Calibration

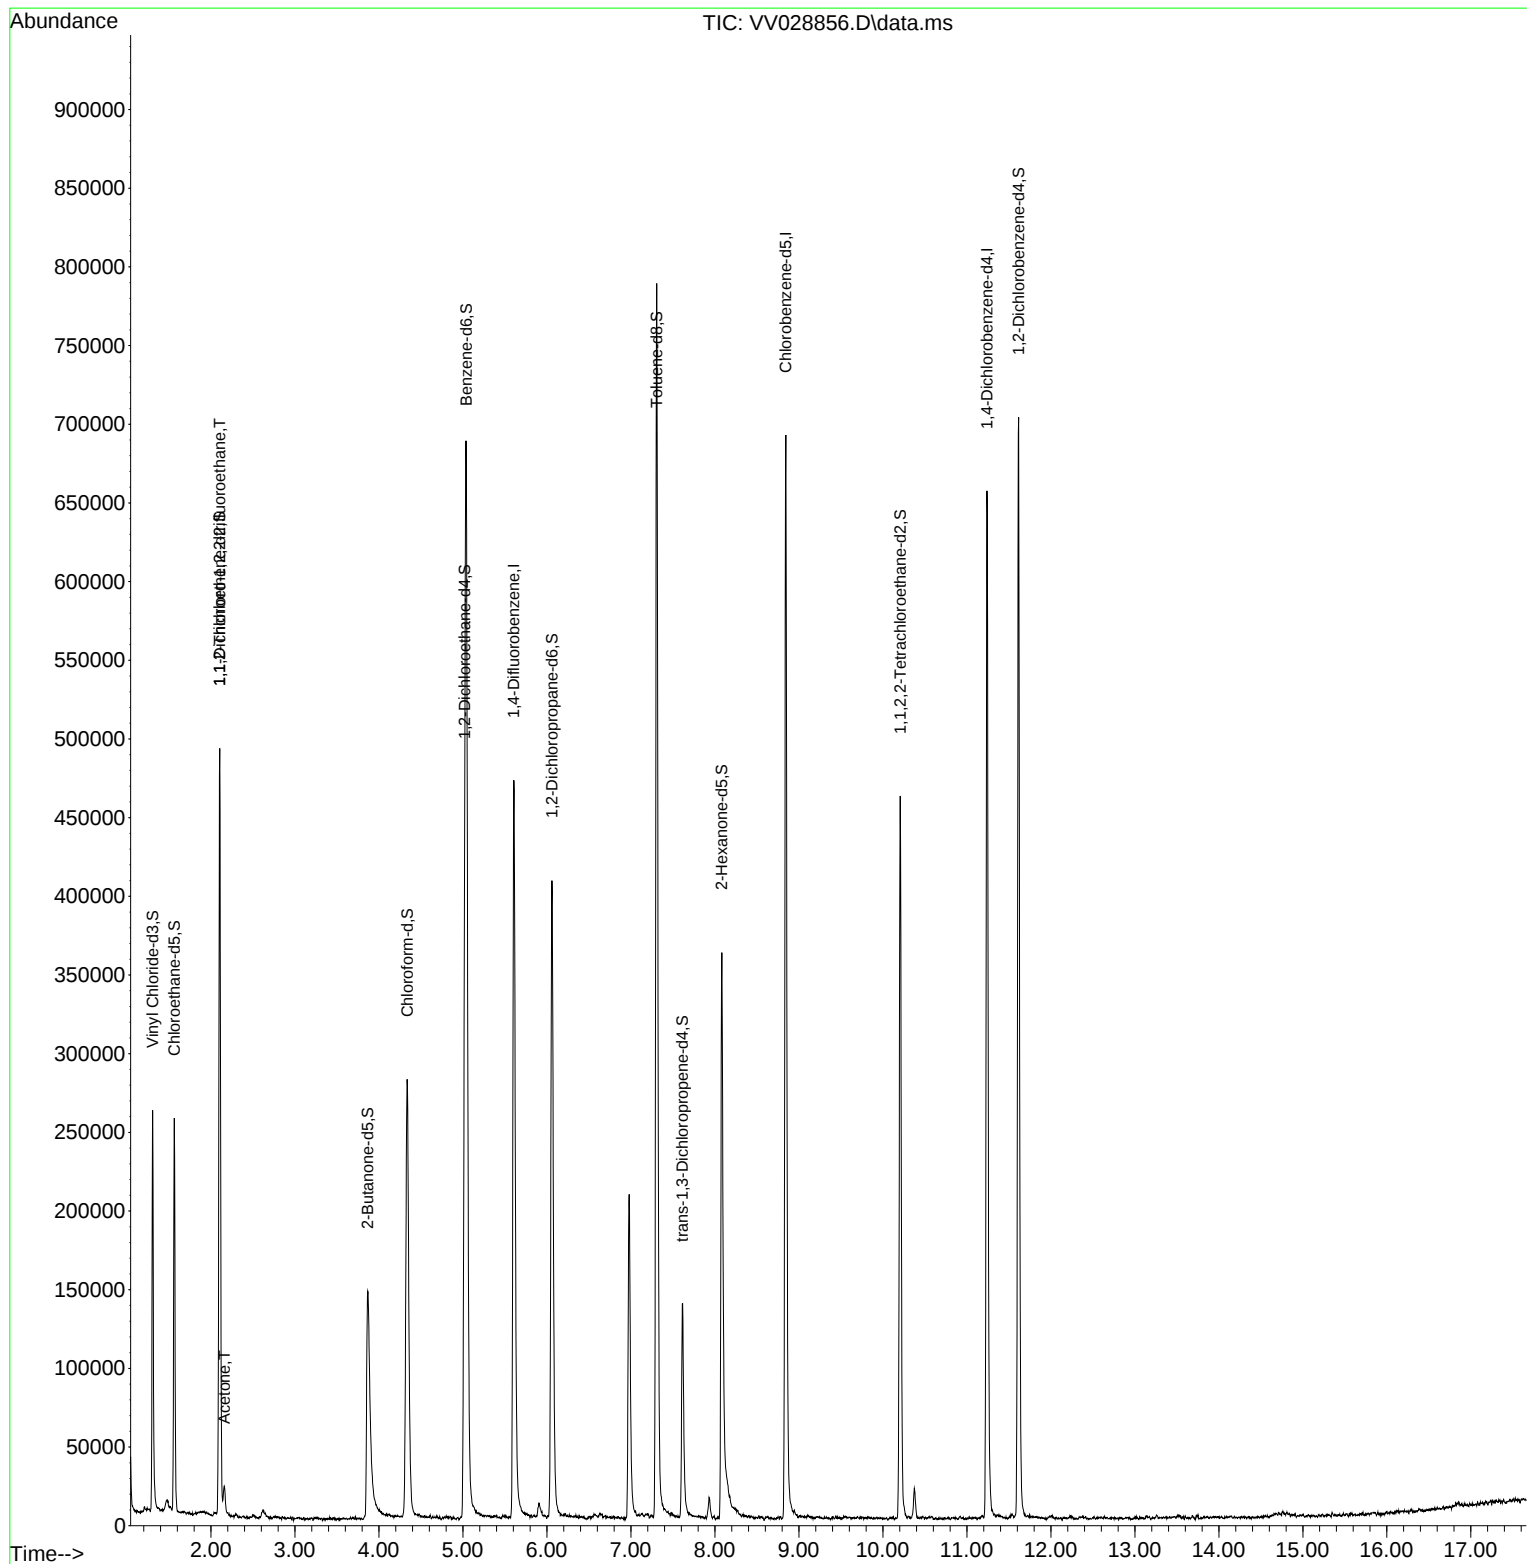

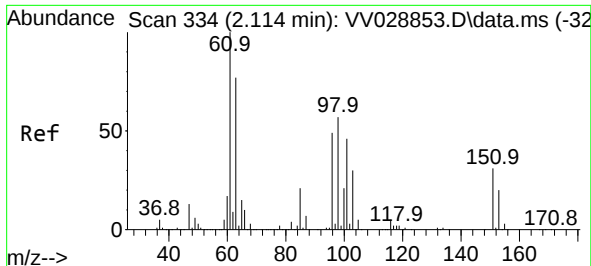

#10

1,1,2-Trichloro-1,2,2-trifluoroethane

Concen: 0.805 ug/L

RT: 2.105 min Scan# 31

Delta R.T. -0.010 min

Lab File: VV028856.D

Acq: 09 Nov 2022 11:09

Instrument :

MSVOA_V

ClientSampleId :

C1122





Tgt Ion:101 Resp: 2324

Ion Ratio Lower Upper

101 100

85 3.2 38.0 57.0#

151 0.0 52.7 79.1#

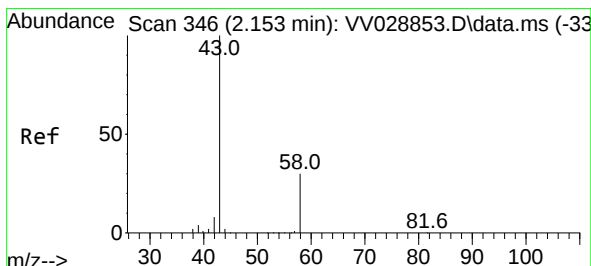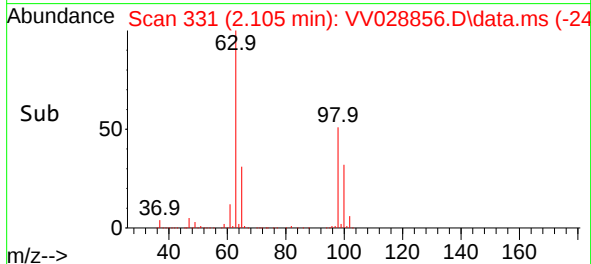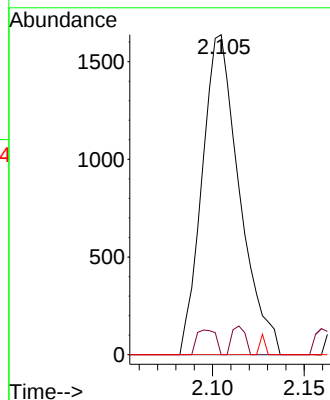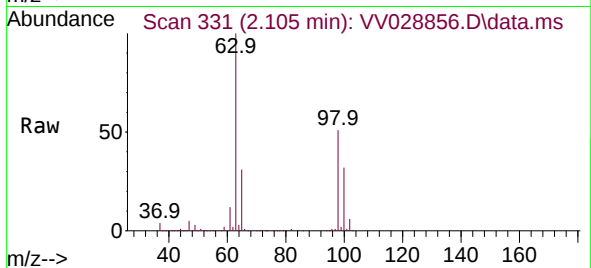

#13

Acetone

Concen: 7.111 ug/L

RT: 2.159 min Scan# 348

Delta R.T. 0.006 min

Lab File: VV028856.D

Acq: 09 Nov 2022 11:09

Tgt Ion: 43 Resp: 18114

Ion Ratio Lower Upper

43 100

58 33.8 0.0 59.0

