

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110922\
 Data File : VV028856.D
 Acq On : 09 Nov 2022 11:09
 Operator : SY/MD
 Sample : N5519-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C1122

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028856.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	102	rBV	253437	281246	15.81%	2.208%
2	1.565	156	163	175	rVB	250183	289273	16.26%	2.271%
3	2.105	321	331	342	rBV	485398	689033	38.73%	5.410%
4	2.748	525	531	533	rBV7	1645	1779	0.10%	0.014%
5	2.847	560	562	567	rBV5	1895	1733	0.10%	0.014%
6	2.973	598	601	605	rVB5	2258	1715	0.10%	0.013%
7	2.992	605	607	609	rBV3	1392	903	0.05%	0.007%
8	3.105	640	642	646	rVB5	1984	1503	0.08%	0.012%
9	3.130	646	650	651	rBV4	1118	740	0.04%	0.006%
10	3.227	676	680	682	rBV4	1710	1068	0.06%	0.008%
11	3.314	704	707	711	rVB5	1374	1261	0.07%	0.010%
12	3.346	711	717	718	rBV5	1446	1178	0.07%	0.009%
13	3.355	718	720	722	rVB3	946	510	0.03%	0.004%
14	3.368	722	724	726	rBV3	976	527	0.03%	0.004%
15	3.423	739	741	743	rVB2	1207	537	0.03%	0.004%
16	3.452	748	750	752	rBV3	1228	703	0.04%	0.006%
17	3.474	755	757	759	rVB3	1316	565	0.03%	0.004%
18	3.503	763	766	767	rBV3	867	460	0.03%	0.004%
19	3.519	767	771	772	rVB4	849	496	0.03%	0.004%
20	3.545	776	779	781	rBV4	1172	847	0.05%	0.007%
21	3.690	818	824	826	rBV6	1406	1337	0.08%	0.010%
22	3.719	831	833	835	rBV3	1833	815	0.05%	0.006%
23	3.751	839	843	846	rBV5	917	664	0.04%	0.005%
24	3.786	852	854	858	rBV5	1007	680	0.04%	0.005%
25	3.867	870	879	920	rBV2	141739	420540	23.64%	3.302%
26	4.336	1012	1025	1053	rVB	276423	675550	37.97%	5.304%
27	4.725	1144	1146	1151	rVB6	2047	1245	0.07%	0.010%
28	4.757	1151	1156	1160	rBV8	1749	1789	0.10%	0.014%
29	4.799	1167	1169	1171	rBV3	1161	560	0.03%	0.004%
30	4.883	1192	1195	1197	rBV4	1410	873	0.05%	0.007%
31	4.941	1207	1213	1215	rBV7	1186	1341	0.08%	0.011%
32	4.973	1217	1223	1224	rBV4	1951	1716	0.10%	0.013%
33	5.037	1227	1243	1271	rBV2	683932	1779068	100.00%	13.967%
34	5.545	1399	1401	1402	rBV2	1369	498	0.03%	0.004%
35	5.606	1408	1420	1450	rBV	468687	957678	53.83%	7.519%
36	6.060	1549	1561	1585	rBV	403997	831747	46.75%	6.530%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110922\
 Data File : VV028856.D
 Acq On : 09 Nov 2022 11:09
 Operator : SY/MD
 Sample : N5519-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C1122

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	6.384	1660	1662	1665	rBV4	2083	1369	0.08%	0.011%
38	6.809	1792	1794	1796	rBV3	1468	749	0.04%	0.006%
39	6.889	1816	1819	1823	rBV7	1149	720	0.04%	0.006%
40	6.928	1829	1831	1833	rBV3	1645	823	0.05%	0.006%
41	6.979	1837	1847	1869	rVV	205660	382501	21.50%	3.003%
42	7.307	1937	1949	1970	rBV	784286	1376105	77.35%	10.804%
43	7.616	2036	2045	2065	rBV	133664	232272	13.06%	1.824%
44	8.037	2173	2176	2180	rVB5	1657	1036	0.06%	0.008%
45	8.082	2180	2190	2219	rBV	359937	717826	40.35%	5.636%
46	8.487	2313	2316	2321	rBV7	1159	1268	0.07%	0.010%
47	8.539	2331	2332	2334	rBV2	1093	495	0.03%	0.004%
48	8.603	2347	2352	2353	rBV4	2192	1643	0.09%	0.013%
49	8.709	2381	2385	2387	rVB5	1075	740	0.04%	0.006%
50	8.780	2403	2407	2411	rBV7	1799	1738	0.10%	0.014%
51	8.844	2416	2427	2453	rBV	687949	1139843	64.07%	8.949%
52	9.162	2524	2526	2528	rVB3	1274	487	0.03%	0.004%
53	9.172	2528	2529	2532	rBV3	1203	752	0.04%	0.006%
54	9.204	2535	2539	2541	rBV5	1342	1075	0.06%	0.008%
55	9.358	2585	2587	2591	rVB4	915	696	0.04%	0.005%
56	9.436	2609	2611	2617	rVB6	1342	960	0.05%	0.008%
57	9.532	2639	2641	2644	rBV4	1605	824	0.05%	0.006%
58	9.728	2700	2702	2704	rBV3	1474	726	0.04%	0.006%
59	9.780	2716	2718	2719	rBV3	1038	452	0.03%	0.004%
60	9.924	2757	2763	2767	rBV8	1235	1152	0.06%	0.009%
61	9.940	2767	2768	2771	rBV3	869	461	0.03%	0.004%
62	10.066	2805	2807	2811	rBV5	1061	975	0.05%	0.008%
63	10.117	2820	2823	2824	rBV3	1092	469	0.03%	0.004%
64	10.149	2829	2833	2835	rBV5	1293	858	0.05%	0.007%
65	10.207	2839	2851	2877	rVV	459084	740962	41.65%	5.817%
66	10.474	2930	2934	2937	rBV5	1456	1332	0.07%	0.010%
67	10.529	2949	2951	2953	rBV3	849	496	0.03%	0.004%
68	10.632	2979	2983	2984	rBV4	1175	787	0.04%	0.006%
69	10.731	3011	3014	3016	rBV4	1292	1001	0.06%	0.008%
70	10.789	3030	3032	3036	rVB4	1302	647	0.04%	0.005%
71	10.815	3037	3040	3041	rBV3	1164	624	0.04%	0.005%
72	10.863	3054	3055	3057	rBV3	1175	495	0.03%	0.004%
73	10.985	3091	3093	3096	rVB3	1238	688	0.04%	0.005%
74	11.008	3097	3100	3103	rBV4	1070	733	0.04%	0.006%
75	11.027	3103	3106	3108	rBV3	1539	877	0.05%	0.007%
76	11.133	3136	3139	3141	rBV4	949	728	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110922\
 Data File : VV028856.D
 Acq On : 09 Nov 2022 11:09
 Operator : SY/MD
 Sample : N5519-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C1122

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	11.239	3161	3172	3197	rBV	652288	1039746	58.44%	8.163%
78	11.522	3258	3260	3261	rBV2	1772	648	0.04%	0.005%
79	11.616	3278	3289	3311	rVB	697948	1106353	62.19%	8.686%
80	11.747	3328	3330	3333	rBV4	2113	947	0.05%	0.007%
81	11.950	3391	3393	3395	rBV3	1208	689	0.04%	0.005%
82	12.059	3424	3427	3429	rBV3	1310	962	0.05%	0.008%
83	12.117	3442	3445	3451	rVB6	1633	1538	0.09%	0.012%
84	12.146	3451	3454	3456	rBV4	1528	1139	0.06%	0.009%
85	12.275	3492	3494	3497	rVB3	1029	467	0.03%	0.004%
86	12.300	3499	3502	3506	rVV5	875	641	0.04%	0.005%
87	12.561	3582	3583	3586	rBV2	1311	740	0.04%	0.006%
88	12.725	3632	3634	3635	rBV2	1304	478	0.03%	0.004%
89	12.757	3642	3644	3645	rBV2	1371	583	0.03%	0.005%
90	12.818	3659	3663	3664	rBV3	1648	1205	0.07%	0.009%
91	12.937	3698	3700	3704	rVB4	1446	927	0.05%	0.007%
92	13.001	3718	3720	3723	rVB5	1191	616	0.03%	0.005%
93	13.056	3734	3737	3741	rBV5	1733	1292	0.07%	0.010%
94	13.204	3779	3783	3784	rBV3	1260	987	0.06%	0.008%
95	13.246	3793	3796	3797	rBV3	1008	580	0.03%	0.005%
96	13.599	3903	3906	3907	rBV4	2430	1480	0.08%	0.012%
97	13.731	3944	3947	3950	rBV5	2417	2175	0.12%	0.017%
98	14.072	4051	4053	4055	rBV3	1386	655	0.04%	0.005%
99	14.265	4110	4113	4115	rBV4	1440	995	0.06%	0.008%
100	14.529	4193	4195	4197	rBV3	1729	913	0.05%	0.007%




Sum of corrected areas: 12737319

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110922\
Data File : VV028856.D
Acq On : 09 Nov 2022 11:09
Operator : SY/MD
Sample : N5519-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C1122

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

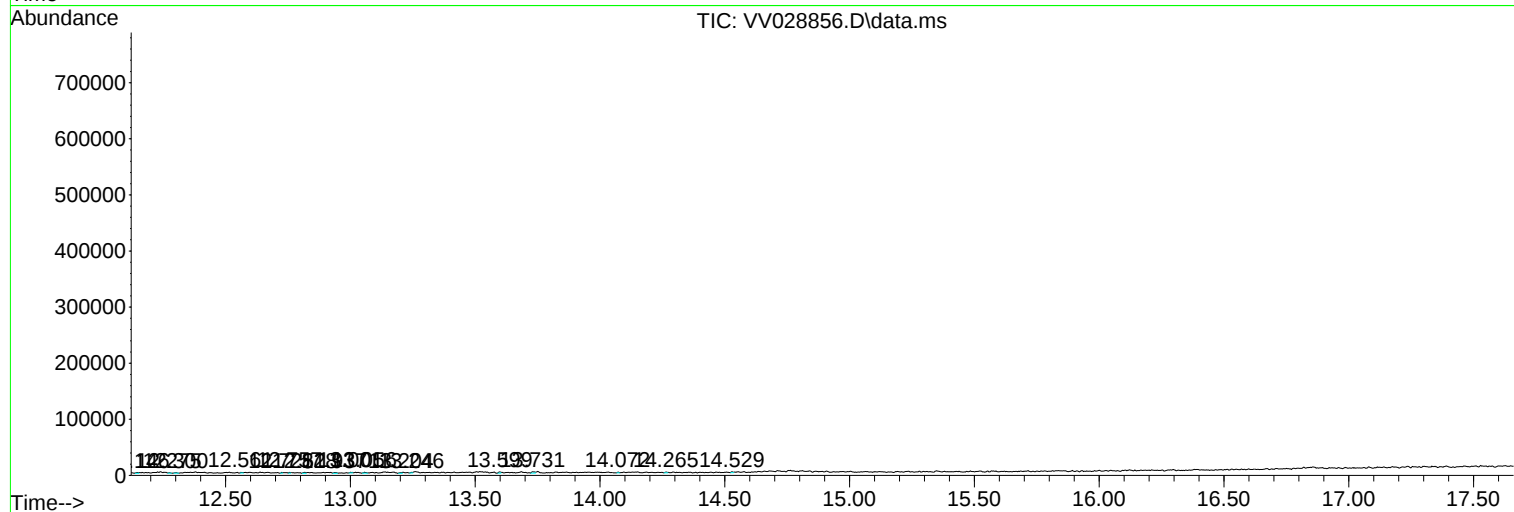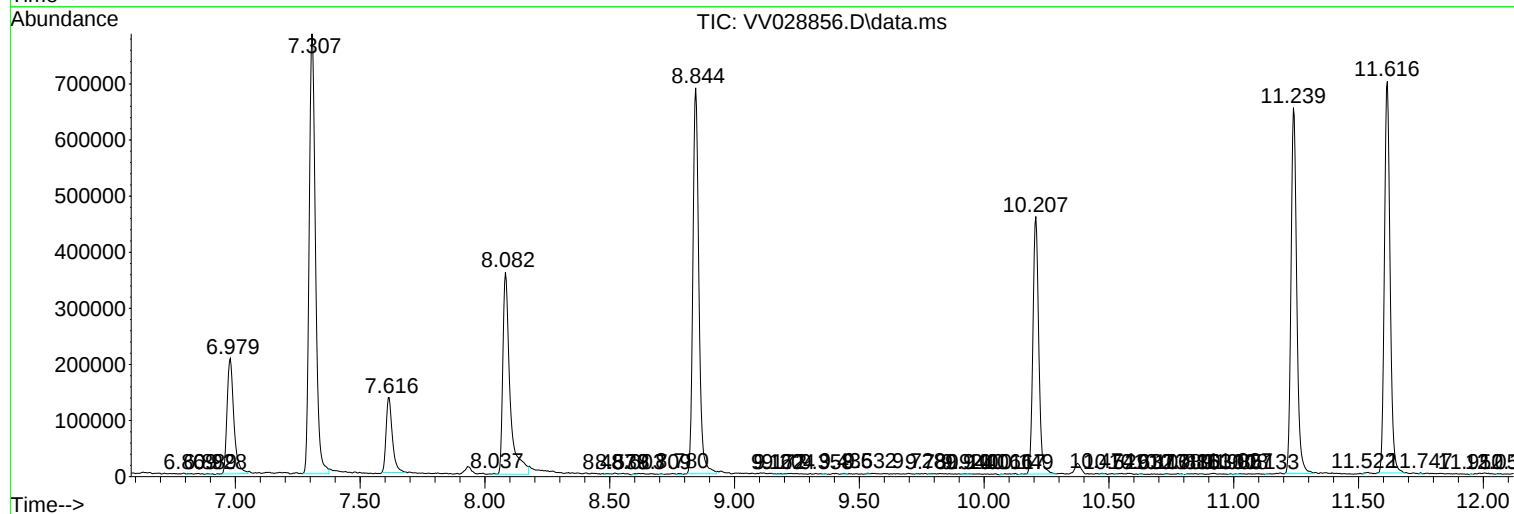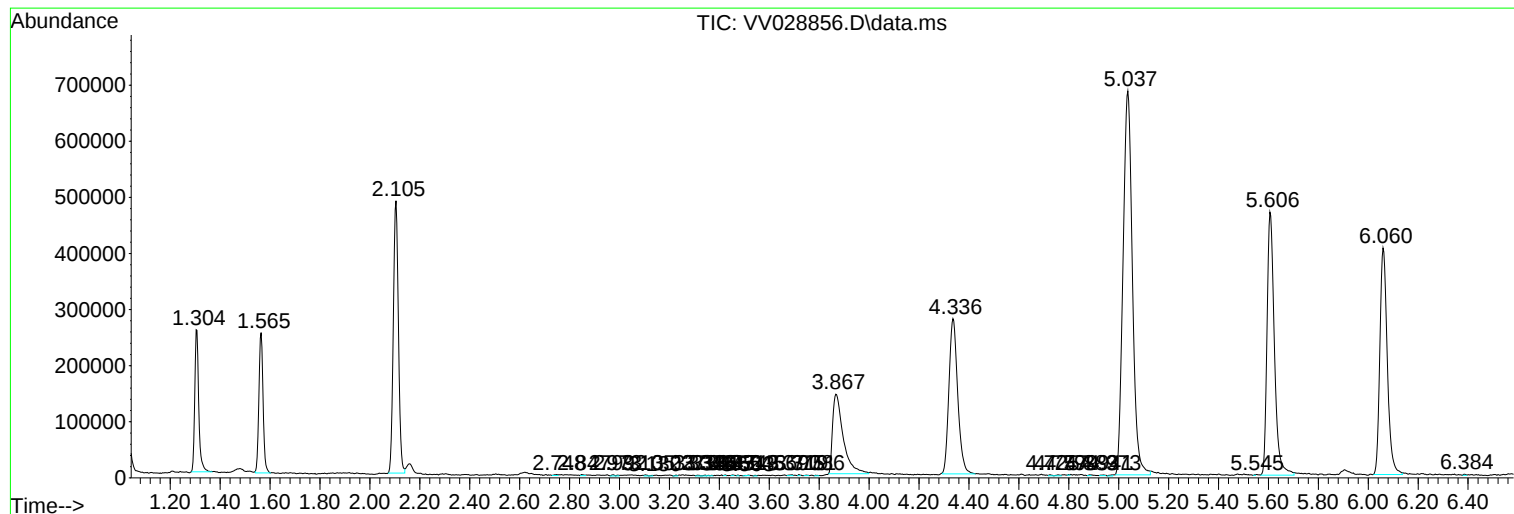

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110922\
Data File : VV028856.D
Acq On : 09 Nov 2022 11:09
Operator : SY/MD
Sample : N5519-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C1122

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110922\
Data File : VV028856.D
Acq On : 09 Nov 2022 11:09
Operator : SY/MD
Sample : N5519-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C1122

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------