

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110922\
 Data File : VV028857.D
 Acq On : 09 Nov 2022 12:25
 Operator : SY/MD
 Sample : N5519-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

Signal : TIC: VV028857.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	111	rVB	265779	292444	16.19%	2.245%
2	1.565	156	163	175	rVB	250314	293336	16.24%	2.252%
3	2.105	321	331	344	rBV	497024	709538	39.28%	5.448%
4	2.413	424	427	428	rBV3	1217	635	0.04%	0.005%
5	2.880	568	572	573	rBV4	899	578	0.03%	0.004%
6	2.892	573	576	578	rBV4	1116	653	0.04%	0.005%
7	2.915	582	583	585	rBV2	1459	715	0.04%	0.005%
8	2.992	606	607	610	rBV2	904	482	0.03%	0.004%
9	3.044	621	623	626	rVB4	1964	755	0.04%	0.006%
10	3.108	639	643	648	rBV7	1550	1775	0.10%	0.014%
11	3.349	715	718	720	rBV3	2273	1778	0.10%	0.014%
12	3.436	742	745	750	rBV7	1017	1160	0.06%	0.009%
13	3.500	763	765	769	rBV5	846	659	0.04%	0.005%
14	3.523	769	772	773	rBV3	1066	718	0.04%	0.006%
15	3.552	779	781	784	rBV4	1436	865	0.05%	0.007%
16	3.590	791	793	795	rBV3	719	311	0.02%	0.002%
17	3.638	806	808	811	rBV4	1121	593	0.03%	0.005%
18	3.683	820	822	824	rBV3	1052	529	0.03%	0.004%
19	3.699	824	827	829	rVV4	930	613	0.03%	0.005%
20	3.761	843	846	848	rBV4	1404	769	0.04%	0.006%
21	3.867	868	879	913	rBV	127422	378313	20.94%	2.905%
22	4.336	1009	1025	1056	rBV	279034	700240	38.77%	5.377%
23	4.773	1159	1161	1162	rBV2	966	413	0.02%	0.003%
24	4.889	1195	1197	1199	rVB3	1485	638	0.04%	0.005%
25	5.034	1226	1242	1268	rBV2	690179	1806244	100.00%	13.869%
26	5.561	1402	1406	1408	rBV5	1524	1210	0.07%	0.009%
27	5.606	1409	1420	1445	rVV	482313	977476	54.12%	7.505%
28	6.060	1549	1561	1594	rBV	411678	843819	46.72%	6.479%
29	6.204	1602	1606	1608	rBV5	2391	1933	0.11%	0.015%
30	6.908	1822	1825	1831	rVB7	1536	1378	0.08%	0.011%
31	6.941	1831	1835	1836	rBV4	1796	1067	0.06%	0.008%
32	6.979	1836	1847	1872	rBV	207428	396013	21.92%	3.041%
33	7.307	1938	1949	1979	rBV	794655	1406246	77.85%	10.797%
34	7.613	2035	2044	2065	rBV	134665	247511	13.70%	1.900%
35	7.876	2124	2126	2130	rBV4	1256	838	0.05%	0.006%
36	8.082	2181	2190	2225	rBV	384907	781427	43.26%	6.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110922\
 Data File : VV028857.D
 Acq On : 09 Nov 2022 12:25
 Operator : SY/MD
 Sample : N5519-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

37	8.670	2369	2373	2375	rBV5	1693	1578	0.09%	0.012%
38	8.693	2379	2380	2381	rBV	1013	273	0.02%	0.002%
39	8.738	2393	2394	2395	rBV	1035	346	0.02%	0.003%
40	8.844	2416	2427	2451	rBV	699862	1168705	64.70%	8.974%
41	9.500	2629	2631	2635	rBV5	1193	649	0.04%	0.005%
42	9.538	2641	2643	2645	rBV3	1276	684	0.04%	0.005%
43	9.571	2651	2653	2654	rBV2	1375	688	0.04%	0.005%
44	9.619	2666	2668	2671	rVB3	2777	1612	0.09%	0.012%
45	9.641	2673	2675	2677	rBV3	862	330	0.02%	0.003%
46	9.654	2677	2679	2680	rBV2	1686	566	0.03%	0.004%
47	9.690	2688	2690	2692	rBV3	1164	470	0.03%	0.004%
48	9.725	2698	2701	2703	rVB4	1473	717	0.04%	0.006%
49	9.738	2703	2705	2709	rVB5	1042	471	0.03%	0.004%
50	9.760	2709	2712	2715	rBV5	1255	1012	0.06%	0.008%
51	9.792	2721	2722	2724	rBV2	807	397	0.02%	0.003%
52	9.889	2749	2752	2755	rBV5	1349	1124	0.06%	0.009%
53	9.982	2777	2781	2782	rBV3	979	648	0.04%	0.005%
54	9.998	2782	2786	2791	rBV6	1031	1164	0.06%	0.009%
55	10.207	2839	2851	2873	rBV	480634	771965	42.74%	5.927%
56	10.384	2904	2906	2909	rBV3	1129	680	0.04%	0.005%
57	10.407	2909	2913	2914	rBV4	1688	1333	0.07%	0.010%
58	10.442	2922	2924	2925	rBV2	1601	823	0.05%	0.006%
59	10.529	2946	2951	2952	rBV5	2079	1630	0.09%	0.013%
60	10.670	2992	2995	2997	rVB4	1283	600	0.03%	0.005%
61	10.738	3013	3016	3019	rBV4	1620	1609	0.09%	0.012%
62	10.786	3029	3031	3032	rBV2	971	440	0.02%	0.003%
63	10.892	3062	3064	3066	rBV3	1068	412	0.02%	0.003%
64	11.043	3107	3111	3112	rBV3	1004	631	0.03%	0.005%
65	11.130	3134	3138	3140	rBV5	1397	1066	0.06%	0.008%
66	11.239	3160	3172	3197	rBV	655312	1066742	59.06%	8.191%
67	11.509	3255	3256	3261	rVB5	1425	888	0.05%	0.007%
68	11.532	3261	3263	3266	rBV4	1849	1331	0.07%	0.010%
69	11.616	3277	3289	3309	rBV	697637	1119545	61.98%	8.596%
70	11.786	3340	3342	3344	rBV2	1545	714	0.04%	0.005%
71	11.889	3370	3374	3376	rBV5	1404	1402	0.08%	0.011%
72	12.072	3427	3431	3434	rBV6	2076	1579	0.09%	0.012%
73	12.088	3434	3436	3438	rVV3	1798	943	0.05%	0.007%
74	12.101	3438	3440	3445	rVB6	2409	1799	0.10%	0.014%
75	12.178	3462	3464	3466	rBV2	839	329	0.02%	0.003%
76	12.191	3466	3468	3469	rBV2	1429	470	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110922\
 Data File : VV028857.D
 Acq On : 09 Nov 2022 12:25
 Operator : SY/MD
 Sample : N5519-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis

77	12.317	3505	3507	3508	rBV3	1051	370	0.02%	0.003%
78	12.326	3508	3510	3511	rBV2	886	377	0.02%	0.003%
79	12.432	3538	3543	3545	rBV5	1262	1014	0.06%	0.008%
80	12.715	3627	3631	3633	rBV5	1359	1074	0.06%	0.008%
81	12.770	3647	3648	3652	rBV4	965	730	0.04%	0.006%
82	12.985	3713	3715	3717	rBV3	895	549	0.03%	0.004%
83	13.178	3772	3775	3777	rVV5	1318	775	0.04%	0.006%
84	13.191	3777	3779	3781	rVB3	857	350	0.02%	0.003%
85	13.223	3787	3789	3790	rBV2	935	373	0.02%	0.003%
86	13.403	3840	3845	3847	rBV5	2006	1568	0.09%	0.012%
87	13.574	3896	3898	3901	rBV4	1248	685	0.04%	0.005%
88	13.606	3905	3908	3909	rBV2	1358	868	0.05%	0.007%
89	13.751	3951	3953	3955	rBV3	1414	825	0.05%	0.006%
90	13.950	4011	4015	4017	rBV5	1361	1009	0.06%	0.008%
91	14.149	4074	4077	4079	rBV4	1279	597	0.03%	0.005%
92	14.246	4105	4107	4109	rBV3	1292	704	0.04%	0.005%


Sum of corrected areas: 13023905

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110922\
Data File : VV028857.D
Acq On : 09 Nov 2022 12:25
Operator : SY/MD
Sample : N5519-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

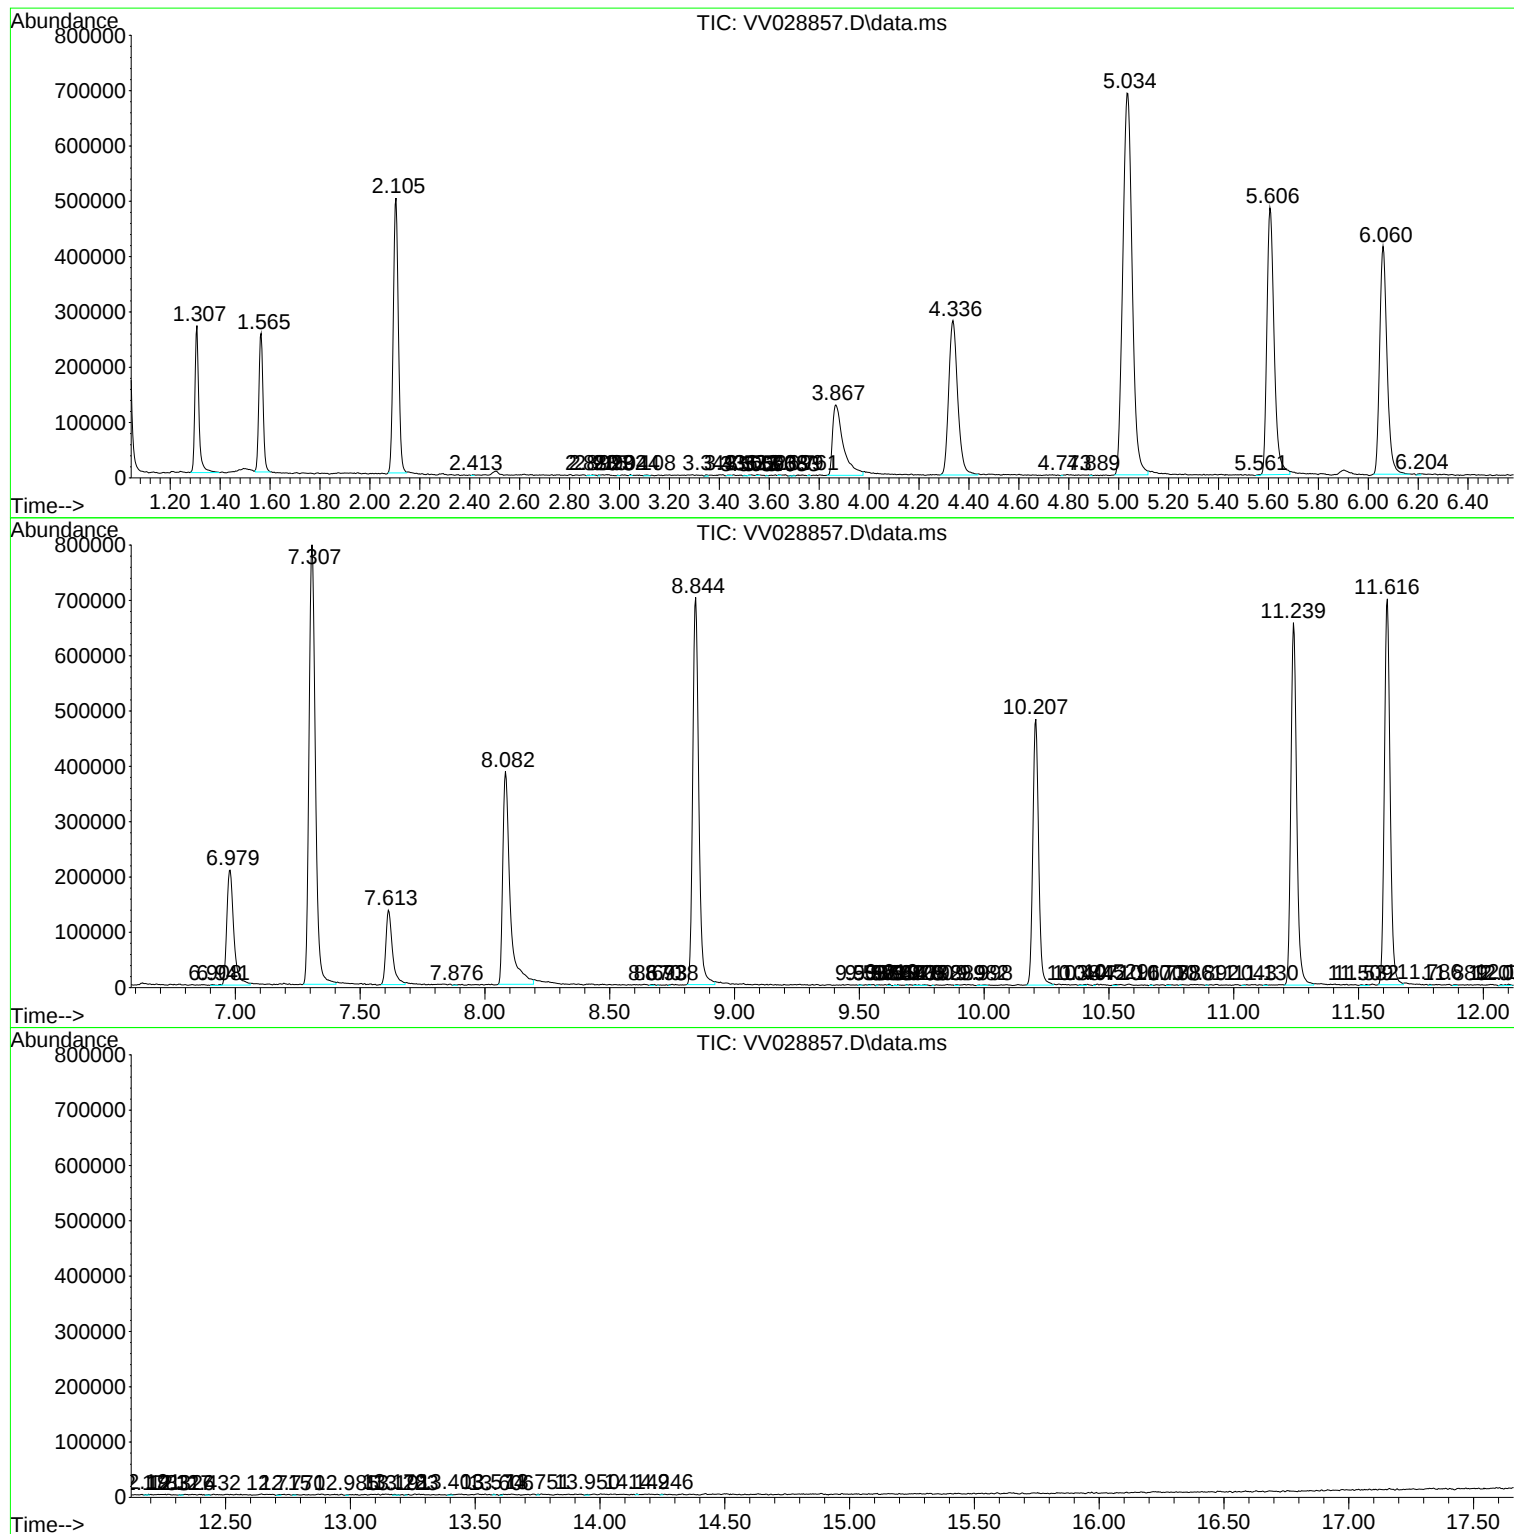

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110922\
Data File : VV028857.D
Acq On : 09 Nov 2022 12:25
Operator : SY/MD
Sample : N5519-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110922\
Data File : VV028857.D
Acq On : 09 Nov 2022 12:25
Operator : SY/MD
Sample : N5519-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc