
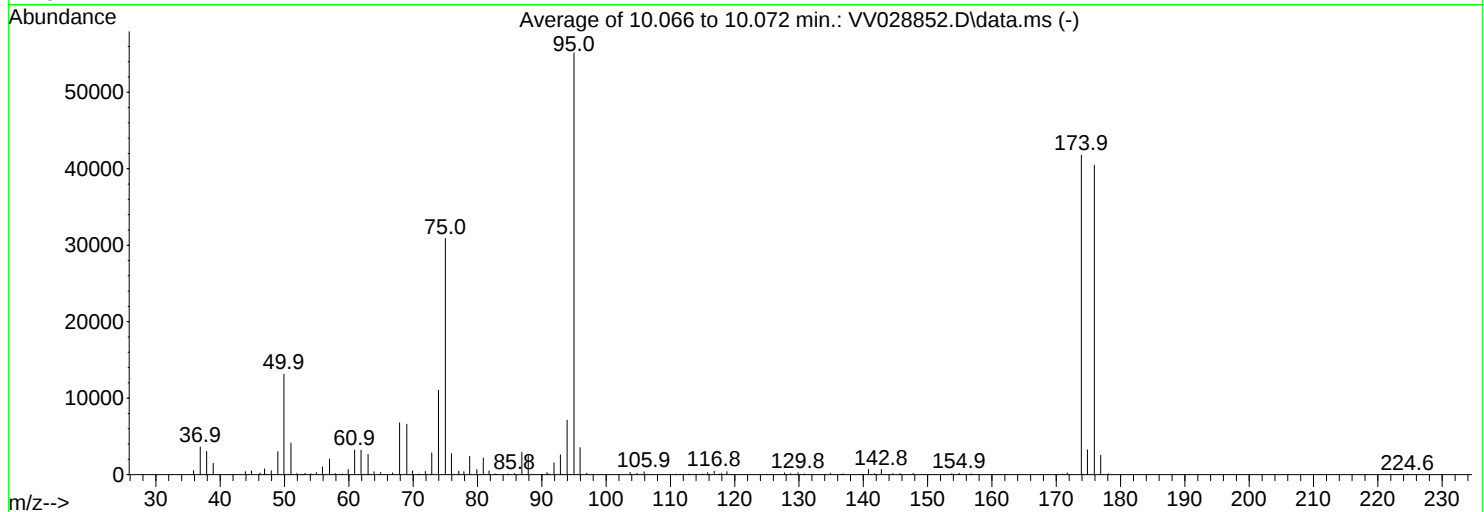


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV110922\
 Data File : VV028852.D
 Acq On : 09 Nov 2022 08:52
 Operator : SY/MD
 Sample : BFB336
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB336

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103122WMA.M
 Title : VOC Analysis
 Last Update : Thu Nov 10 00:43:48 2022

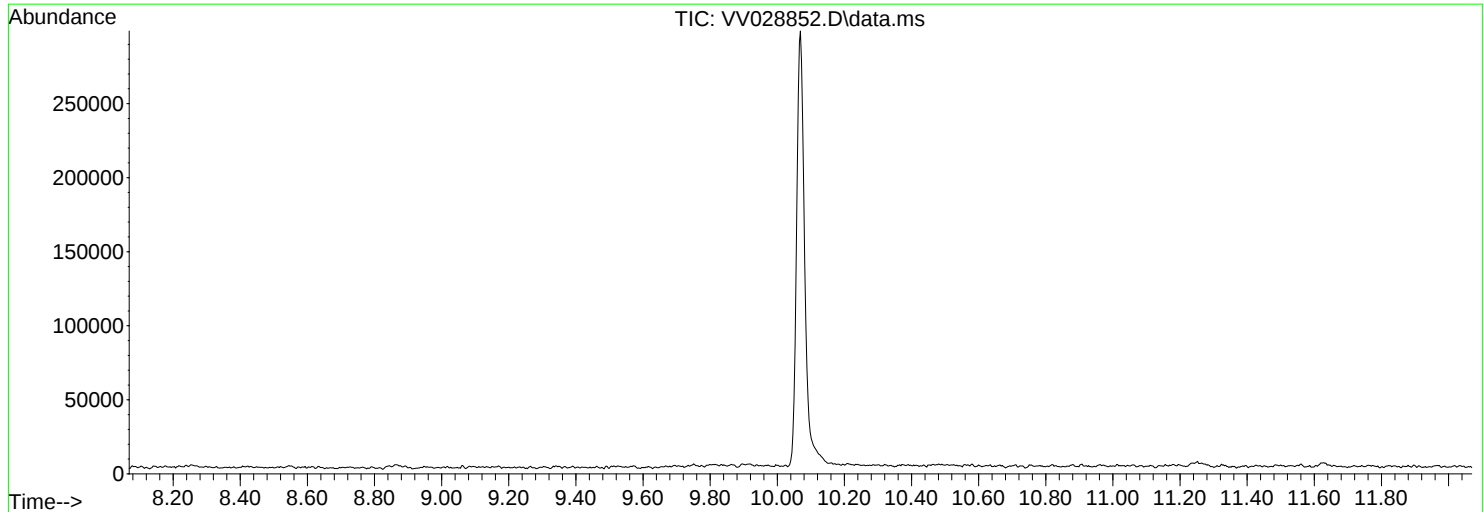

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.8	13137	PASS
75	95	30	80	56.0	30883	PASS
95	95	100	100	100.0	55157	PASS
96	95	5	9	6.4	3540	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.7	41771	PASS
175	174	5	9	7.8	3252	PASS
176	174	95	105	96.9	40461	PASS
177	176	5	10	6.3	2538	PASS

m/z	Abundance
35.90	977.0
36.80	169.0
37.90	446.0
39.80	317.0
40.90	158.0
41.70	155.0
42.50	166.0
43.90	593.0
44.80	134.0
45.50	107.0
47.00	108.0
47.50	135.0
48.50	123.0
49.10	106.0
49.90	137.0
50.40	103.0
51.80	115.0
52.80	125.0
56.40	115.0
62.30	108.0
63.60	115.0
66.10	117.0
70.00	115.0
70.40	112.0
79.40	112.0
80.20	103.0
98.70	118.0
101.90	115.0
106.70	110.0
113.90	101.0
149.40	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB336

m/z	Abundance
35.90	1545.0
36.90	3876.0
37.90	3603.0
38.90	1516.0
39.90	388.0
40.70	162.0
41.70	151.0
42.70	155.0
44.00	1007.0
44.90	589.0
46.20	225.0
46.90	931.0
47.90	572.0
48.90	3075.0
50.00	13425.0
51.00	4324.0
52.00	233.0
52.70	139.0
53.20	169.0
53.90	132.0
54.00	133.0
55.00	241.0
55.90	1082.0
57.00	2156.0
58.00	181.0
58.60	128.0
59.90	649.0
60.90	3172.0
61.90	3125.0
63.00	2746.0
63.90	372.0
64.90	265.0
66.90	258.0
67.90	7177.0
69.00	6905.0
69.90	515.0
71.00	148.0
71.90	488.0
72.90	2929.0
74.00	11256.0
75.00	32064.0
75.90	3036.0
77.10	485.0
77.90	431.0
78.80	2385.0
79.90	606.0
80.90	2019.0
81.80	533.0
82.80	115.0
83.00	118.0
84.70	123.0
85.70	160.0
86.90	2907.0
87.90	2502.0
90.80	251.0
91.90	1668.0
92.90	2623.0
93.90	6955.0
95.00	55608.0
96.00	3669.0
97.00	239.0
103.80	337.0
104.80	146.0
106.00	382.0
111.50	103.0
112.90	122.0
115.80	288.0
116.80	374.0
117.60	238.0
118.80	395.0
127.70	251.0
128.70	136.0
129.80	250.0
130.90	110.0
134.90	182.0
136.60	119.0
139.90	109.0
140.80	648.0
141.70	103.0
142.80	709.0
144.60	122.0
145.70	157.0
147.90	178.0
153.80	121.0
154.90	220.0
156.80	142.0
171.00	144.0
171.70	257.0
173.90	40352.0
174.90	3267.0
175.90	40264.0
176.90	2573.0

Instrument :
MSVOA_V
ClientSampleId :
BFB336

178.10

185.0

Instrument :
MSVOA_V
ClientSampleId :
BFB336

m/z	Abundance
35.90	1511.0
37.00	3885.0
38.00	3593.0
38.90	1541.0
39.90	354.0
40.80	187.0
41.70	138.0
42.70	180.0
43.90	977.0
44.90	631.0
46.20	237.0
46.90	848.0
48.00	534.0
48.90	3245.0
50.00	13735.0
51.00	4234.0
52.00	243.0
52.80	139.0
53.20	173.0
54.10	123.0
55.00	279.0
55.90	1039.0
57.00	2124.0
57.90	143.0
58.90	115.0
59.90	690.0
60.90	3313.0
61.90	3256.0
63.00	2733.0
63.90	408.0
65.00	294.0
66.80	223.0
67.90	7039.0
69.00	6835.0
69.90	664.0
70.90	133.0
71.90	448.0
72.90	2902.0
74.00	11403.0
75.00	31928.0
76.00	2821.0
77.10	498.0
77.90	395.0
78.80	2450.0
79.90	699.0
80.90	2185.0
81.80	530.0
82.70	123.0
84.70	105.0
85.80	160.0
86.90	3057.0
87.90	2671.0
90.80	291.0
91.00	286.0
91.90	1588.0
92.90	2678.0
94.00	7352.0
95.00	56912.0
96.00	3590.0
97.00	203.0
103.80	295.0
104.80	172.0
105.90	380.0
110.90	113.0
112.10	105.0
112.90	119.0
114.90	111.0
115.80	292.0
116.80	479.0
117.90	229.0
118.80	399.0
125.00	108.0
127.70	234.0
128.70	115.0
129.90	257.0
130.80	104.0
134.90	187.0
136.80	131.0
139.90	105.0
140.80	705.0
141.80	121.0
142.80	693.0
144.60	128.0
145.70	161.0
147.70	155.0
153.70	120.0
154.90	198.0
156.70	144.0
171.00	132.0
171.70	216.0
173.90	43312.0
174.90	3322.0

Instrument :
MSVOA_V
ClientSampleId :
BFB336

175.90

176.90

178.10

41904.0

2578.0

134.0

Instrument :

MSVOA_V

ClientSampleId :

BFB336

m/z	Abundance
35.90	1505.0
37.00	3638.0
38.00	3249.0
38.90	1410.0
40.00	341.0
40.90	175.0
41.70	154.0
42.70	154.0
43.90	992.0
44.90	665.0
46.20	200.0
46.90	832.0
48.00	481.0
49.00	3063.0
49.90	12662.0
51.00	3821.0
52.00	243.0
52.80	125.0
53.20	140.0
54.20	115.0
54.90	297.0
55.90	945.0
57.00	1868.0
57.80	127.0
59.00	120.0
59.90	643.0
60.90	3174.0
61.90	3201.0
63.00	2448.0
63.90	365.0
65.00	329.0
65.90	101.0
66.70	194.0
67.90	6148.0
69.00	6052.0
69.90	689.0
71.90	346.0
72.90	2691.0
73.90	10449.0
75.00	28656.0
76.00	2461.0
77.10	422.0
77.90	303.0
78.80	2317.0
79.90	729.0
80.90	2333.0
81.80	477.0
82.80	103.0
85.80	124.0
86.90	2884.0
87.90	2611.0
89.10	111.0
90.80	294.0
91.90	1421.0
92.90	2494.0
94.00	7076.0
95.00	52952.0
95.90	3361.0
97.00	137.0
103.70	264.0
104.80	184.0
105.80	369.0
107.00	111.0
109.90	103.0
110.80	111.0
112.10	111.0
115.00	143.0
115.80	270.0
116.80	538.0
118.00	256.0
118.80	399.0
127.80	214.0
128.70	111.0
129.90	235.0
130.80	108.0
134.90	175.0
136.90	161.0
140.80	660.0
141.80	131.0
142.80	669.0
144.60	130.0
145.70	143.0
147.70	125.0
153.70	109.0
154.90	129.0
156.80	124.0
171.70	232.0
173.90	41648.0
174.80	3167.0
175.90	39216.0
176.90	2462.0
224.60	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB336