

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111020\
 Data File : VV019317.D
 Acq On : 10 Nov 2020 12:28
 Operator : SY/MD
 Sample : L4659-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG498

Quant Time: Nov 11 03:34:19 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 11 02:14:49 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	254026	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	250754	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	118180	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	105585	52.30	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	104.60%
7) Chloroethane-d5	1.58	69	85304	54.39	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	108.78%
11) 1,1-Dichloroethene-d2	2.12	63	157506	41.01	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.02%
21) 2-Butanone-d5	3.91	46	117297	94.87	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	94.87%
24) Chloroform-d	4.37	84	176758	47.07	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.14%
26) 1,2-Dichloroethane-d4	5.06	65	124250	47.48	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.96%
32) Benzene-d6	5.07	84	337915	47.51	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.02%
36) 1,2-Dichloropropane-d6	6.09	67	107103	50.50	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.00%
41) Toluene-d8	7.34	98	300400	43.96	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.92%
43) trans-1,3-Dichloropropene-	7.64	79	53363	43.48	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.96%
47) 2-Hexanone-d5	8.11	63	67923	73.95	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	73.95%
57) 1,1,2,2-Tetrachloroethane-	10.23	84	116816	40.85	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	81.70%
64) 1,2-Dichlorobenzene-d4	11.65	152	120399	48.49	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.98%


Target Compounds					Ovalue
13) Acetone	2.20	43	4012	3.493 ug/L	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111020\
Data File : VV019317.D
Acq On : 10 Nov 2020 12:28
Operator : SY/MD
Sample : L4659-10
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG498

Quant Time: Nov 11 03:34:19 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 11 02:14:49 2020
Response via : Initial Calibration

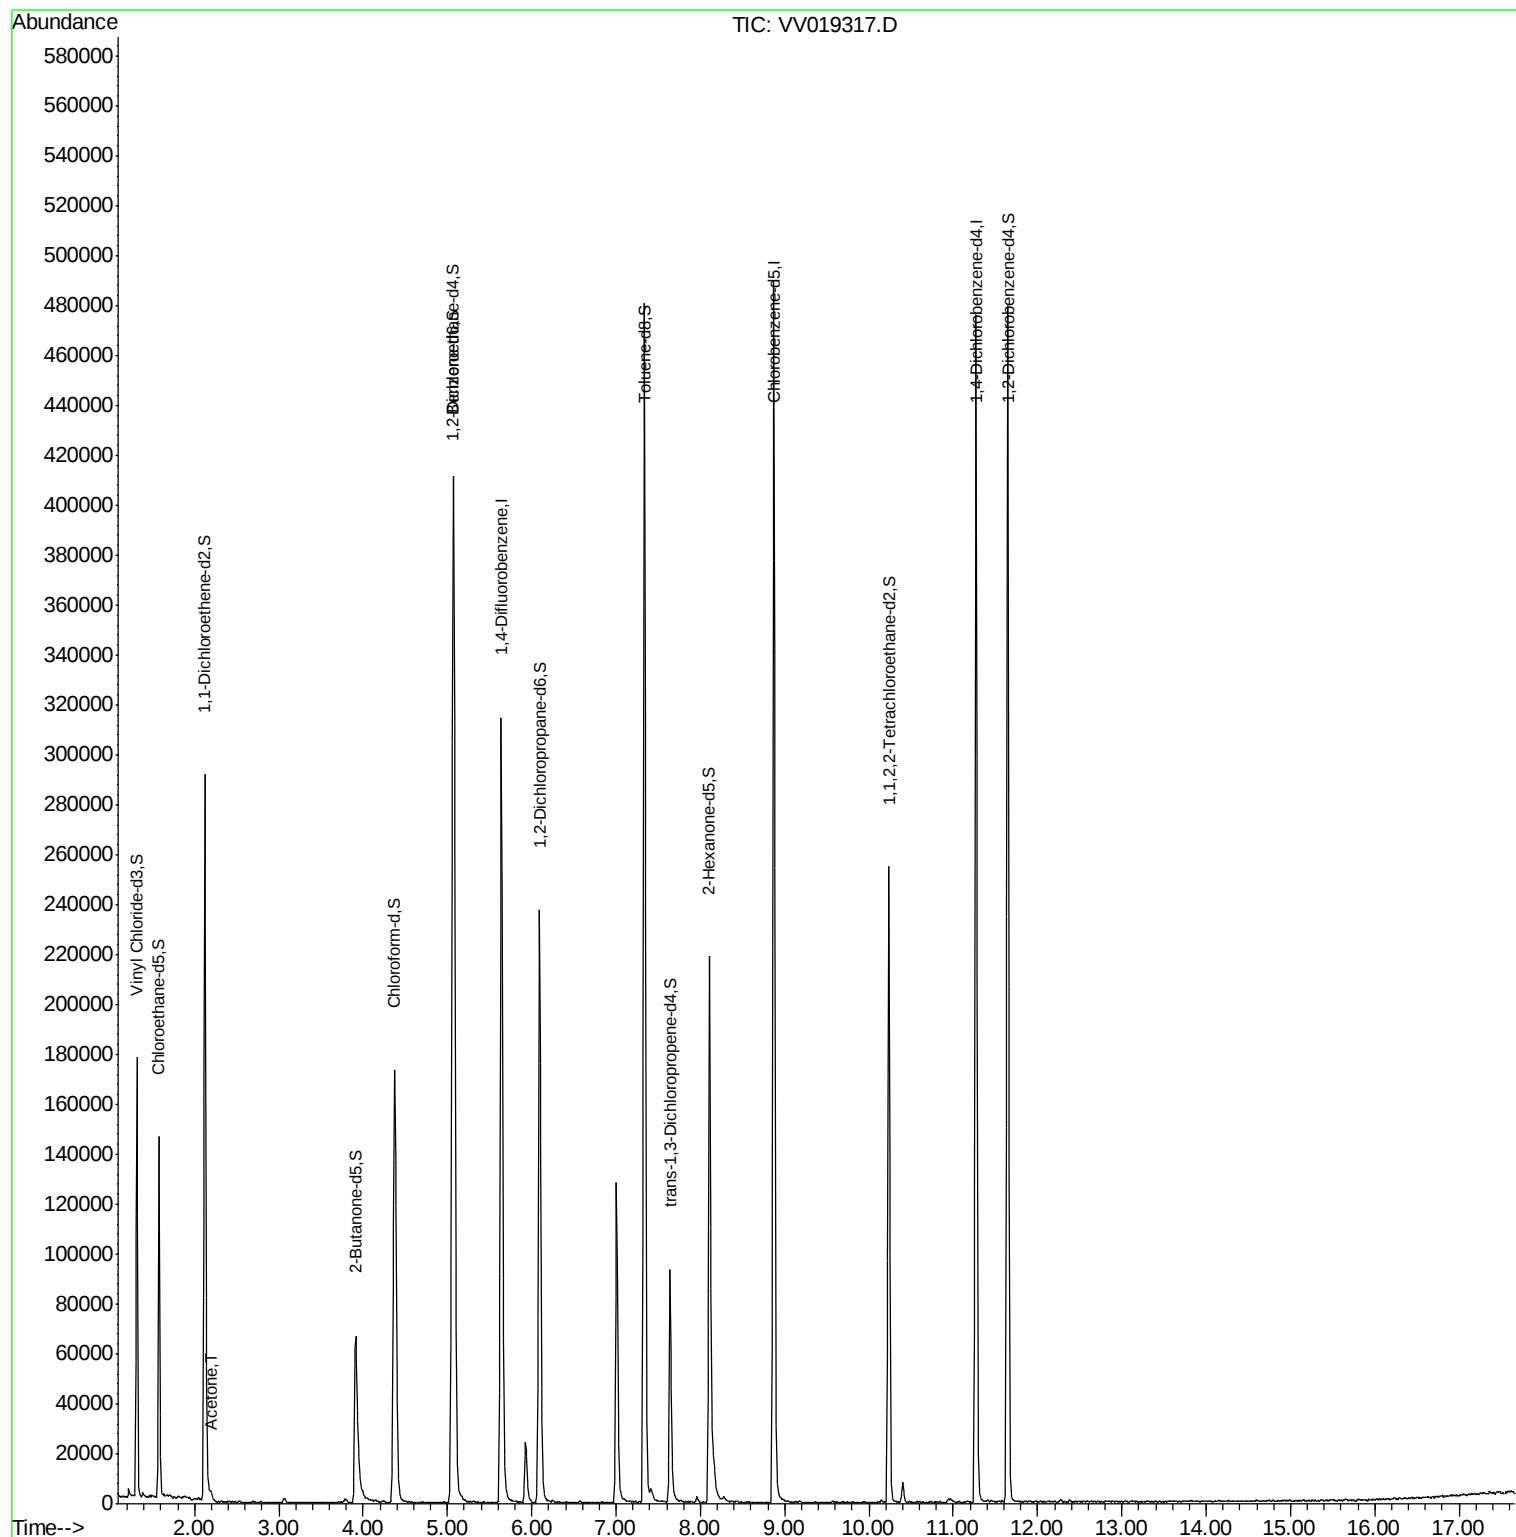

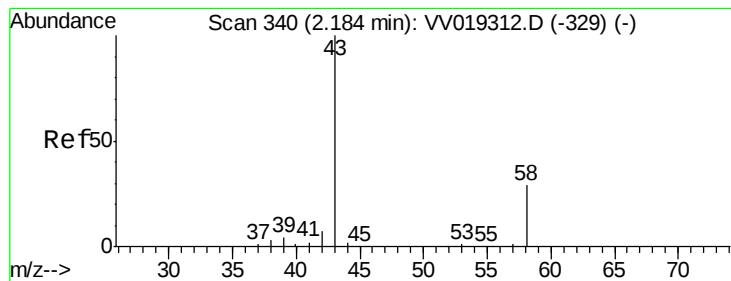

#13
 Acetone
 Concen: 3.493 ug/L
 RT: 2.20 min Scan# 344
 Delta R.T. 0.01 min
 Lab File: VV019317.D
 Acq: 10 Nov 2020 12:28

Instrument :
 MSVOA_V
 ClientSampleId :
 BG498

Tot Ion: 43 Resp: 4012
 Ion Ratio Lower Upper
 43 100
 58 17.7 0.0 59.4

