

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111020\
 Data File : VV019328.D
 Acq On : 10 Nov 2020 17:05
 Operator : SY/MD
 Sample : VIBLK95
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK95

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	63	70	85	rVB	175223	170160	16.23%	2.134%
2	1.579	144	152	165	rBV	142411	159698	15.23%	2.003%
3	1.997	280	282	283	rBV	643	258	0.02%	0.003%
4	2.122	309	321	353	rVB	285196	433724	41.36%	5.440%
5	2.232	353	355	362	rVB3	460	436	0.04%	0.005%
6	2.315	376	381	385	rBV2	461	513	0.05%	0.006%
7	2.524	439	446	455	rBV2	2050	3198	0.30%	0.040%
8	2.730	505	510	513	rBV	282	170	0.02%	0.002%
9	2.878	552	556	558	rBV	274	178	0.02%	0.002%
10	3.235	659	667	672	rVB2	175	261	0.02%	0.003%
11	3.264	672	676	681	rBV3	214	212	0.02%	0.003%
12	3.534	755	760	763	rBV2	193	181	0.02%	0.002%
13	3.917	868	879	920	rBV	64959	212300	20.24%	2.663%
14	4.261	982	986	990	rBV2	352	354	0.03%	0.004%
15	4.376	1003	1022	1054	rVV	171169	421052	40.15%	5.281%
16	4.560	1075	1079	1082	rBV3	271	250	0.02%	0.003%
17	4.685	1115	1118	1122	rBV	465	310	0.03%	0.004%
18	4.714	1122	1127	1129	rVV2	216	166	0.02%	0.002%
19	4.733	1131	1133	1137	rVB2	264	173	0.02%	0.002%
20	4.868	1173	1175	1180	rVB	246	174	0.02%	0.002%
21	4.997	1213	1215	1219	rBV	265	180	0.02%	0.002%
22	5.071	1221	1238	1266	rBV2	410440	1048703	100.00%	13.153%
23	5.428	1347	1349	1352	rBV	303	203	0.02%	0.003%
24	5.511	1363	1375	1377	rBV2	464	616	0.06%	0.008%
25	5.524	1377	1379	1384	rVB3	383	264	0.03%	0.003%
26	5.640	1402	1415	1449	rBV	308777	623269	59.43%	7.817%
27	5.817	1467	1470	1474	rBV3	310	295	0.03%	0.004%
28	5.862	1482	1484	1488	rVB2	326	214	0.02%	0.003%
29	5.929	1494	1505	1519	rBV2	17955	37072	3.54%	0.465%
30	6.007	1527	1529	1533	rVB2	257	170	0.02%	0.002%
31	6.048	1539	1542	1543	rBV	555	315	0.03%	0.004%
32	6.093	1543	1556	1578	rBV	233791	476203	45.41%	5.973%
33	6.235	1597	1600	1601	rBV2	535	324	0.03%	0.004%
34	6.280	1610	1614	1617	rBV2	264	232	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111020\
 Data File : VV019328.D
 Acq On : 10 Nov 2020 17:05
 Operator : SY/MD
 Sample : VIBLK95
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK95

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

35	6.396	1646	1650	1652	rBV	275	187	0.02%	0.002%
36	6.653	1728	1730	1734	rBV2	294	250	0.02%	0.003%
37	6.701	1742	1745	1750	rBV2	216	188	0.02%	0.002%
38	7.006	1829	1840	1867	rBV2	129579	232566	22.18%	2.917%
39	7.170	1888	1891	1893	rBV2	339	209	0.02%	0.003%
40	7.241	1909	1913	1917	rVB4	501	428	0.04%	0.005%
41	7.261	1917	1919	1921	rVB	438	207	0.02%	0.003%
42	7.280	1921	1925	1927	rBV2	346	223	0.02%	0.003%
43	7.338	1931	1943	1962	rBV	475739	810929	77.33%	10.171%
44	7.521	1997	2000	2004	rVB3	761	522	0.05%	0.007%
45	7.643	2026	2038	2066	rBV	92010	165442	15.78%	2.075%
46	7.842	2097	2100	2102	rBV2	260	167	0.02%	0.002%
47	7.859	2102	2105	2110	rVV4	352	351	0.03%	0.004%
48	7.887	2110	2114	2119	rVV3	372	411	0.04%	0.005%
49	7.933	2125	2128	2132	rVV2	299	216	0.02%	0.003%
50	7.997	2142	2148	2161	rBV5	4414	7094	0.68%	0.089%
51	8.109	2170	2183	2221	rBV2	232412	456521	43.53%	5.726%
52	8.322	2247	2249	2251	rBV2	322	189	0.02%	0.002%
53	8.367	2259	2263	2266	rVB2	373	251	0.02%	0.003%
54	8.482	2295	2299	2301	rBV	330	211	0.02%	0.003%
55	8.498	2301	2304	2307	rVB2	315	217	0.02%	0.003%
56	8.518	2307	2310	2312	rBV2	271	181	0.02%	0.002%
57	8.576	2324	2328	2330	rBV2	325	201	0.02%	0.003%
58	8.733	2374	2377	2380	rBV2	258	189	0.02%	0.002%
59	8.871	2408	2420	2449	rBV	478858	783811	74.74%	9.831%
60	9.084	2483	2486	2490	rVB	295	193	0.02%	0.002%
61	9.135	2499	2502	2506	rVB3	292	236	0.02%	0.003%
62	9.167	2506	2512	2519	rBV4	476	651	0.06%	0.008%
63	9.222	2525	2529	2531	rBV2	276	201	0.02%	0.003%
64	9.389	2578	2581	2584	rBV2	291	223	0.02%	0.003%
65	9.543	2626	2629	2632	rVV2	268	188	0.02%	0.002%
66	9.685	2671	2673	2678	rVB	295	207	0.02%	0.003%
67	9.865	2725	2729	2736	rVB2	370	475	0.05%	0.006%
68	9.903	2736	2741	2744	rBV2	402	328	0.03%	0.004%
69	10.145	2808	2816	2818	rBV3	794	982	0.09%	0.012%
70	10.235	2832	2844	2863	rBV	271132	433941	41.38%	5.443%
71	10.350	2877	2880	2883	rVB	311	205	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111020\
 Data File : VV019328.D
 Acq On : 10 Nov 2020 17:05
 Operator : SY/MD
 Sample : VIBLK95
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK95

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis

72	10.373	2883	2887	2889	rBV2	247	171	0.02%	0.002%
73	10.444	2904	2909	2913	rBV2	249	218	0.02%	0.003%
74	10.907	3048	3053	3056	rBV2	328	381	0.04%	0.005%
75	10.929	3056	3060	3062	rBV3	437	344	0.03%	0.004%
76	11.006	3081	3084	3087	rBV2	342	218	0.02%	0.003%
77	11.167	3131	3134	3136	rBV2	373	265	0.03%	0.003%
78	11.270	3154	3166	3185	rBV	479633	724816	69.12%	9.091%
79	11.492	3231	3235	3238	rBV2	265	207	0.02%	0.003%
80	11.556	3249	3255	3259	rBV3	388	446	0.04%	0.006%
81	11.595	3265	3267	3271	rVB2	243	172	0.02%	0.002%
82	11.646	3271	3283	3308	rBV	478599	749204	71.44%	9.397%
83	11.823	3332	3338	3341	rBV3	513	540	0.05%	0.007%
84	11.929	3367	3371	3377	rBV2	285	342	0.03%	0.004%
85	12.042	3403	3406	3408	rBV	222	167	0.02%	0.002%
86	12.231	3461	3465	3468	rBV2	321	296	0.03%	0.004%
87	12.283	3478	3481	3488	rVB3	400	360	0.03%	0.005%
88	12.447	3529	3532	3535	rBV2	313	182	0.02%	0.002%
89	12.614	3581	3584	3588	rBV	311	276	0.03%	0.003%
90	12.755	3625	3628	3632	rBV2	292	275	0.03%	0.003%
91	12.881	3664	3667	3671	rBV	394	301	0.03%	0.004%
92	13.492	3852	3857	3861	rBV2	286	210	0.02%	0.003%
93	13.714	3923	3926	3928	rBV2	318	218	0.02%	0.003%
94	14.125	4051	4054	4057	rBV2	407	316	0.03%	0.004%
95	14.222	4082	4084	4089	rVB2	404	277	0.03%	0.003%
96	14.714	4234	4237	4240	rVB	376	168	0.02%	0.002%
97	14.733	4240	4243	4246	rBV	400	354	0.03%	0.004%
98	15.170	4376	4379	4381	rBV2	489	317	0.03%	0.004%
99	15.659	4527	4531	4536	rVB3	550	554	0.05%	0.007%
100	15.794	4571	4573	4579	rVB3	800	473	0.05%	0.006%


Sum of corrected areas: 7972887

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV111020\
Data File : VV019328.D
Acq On : 10 Nov 2020 17:05
Operator : SY/MD
Sample : VIBLK95
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK95

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

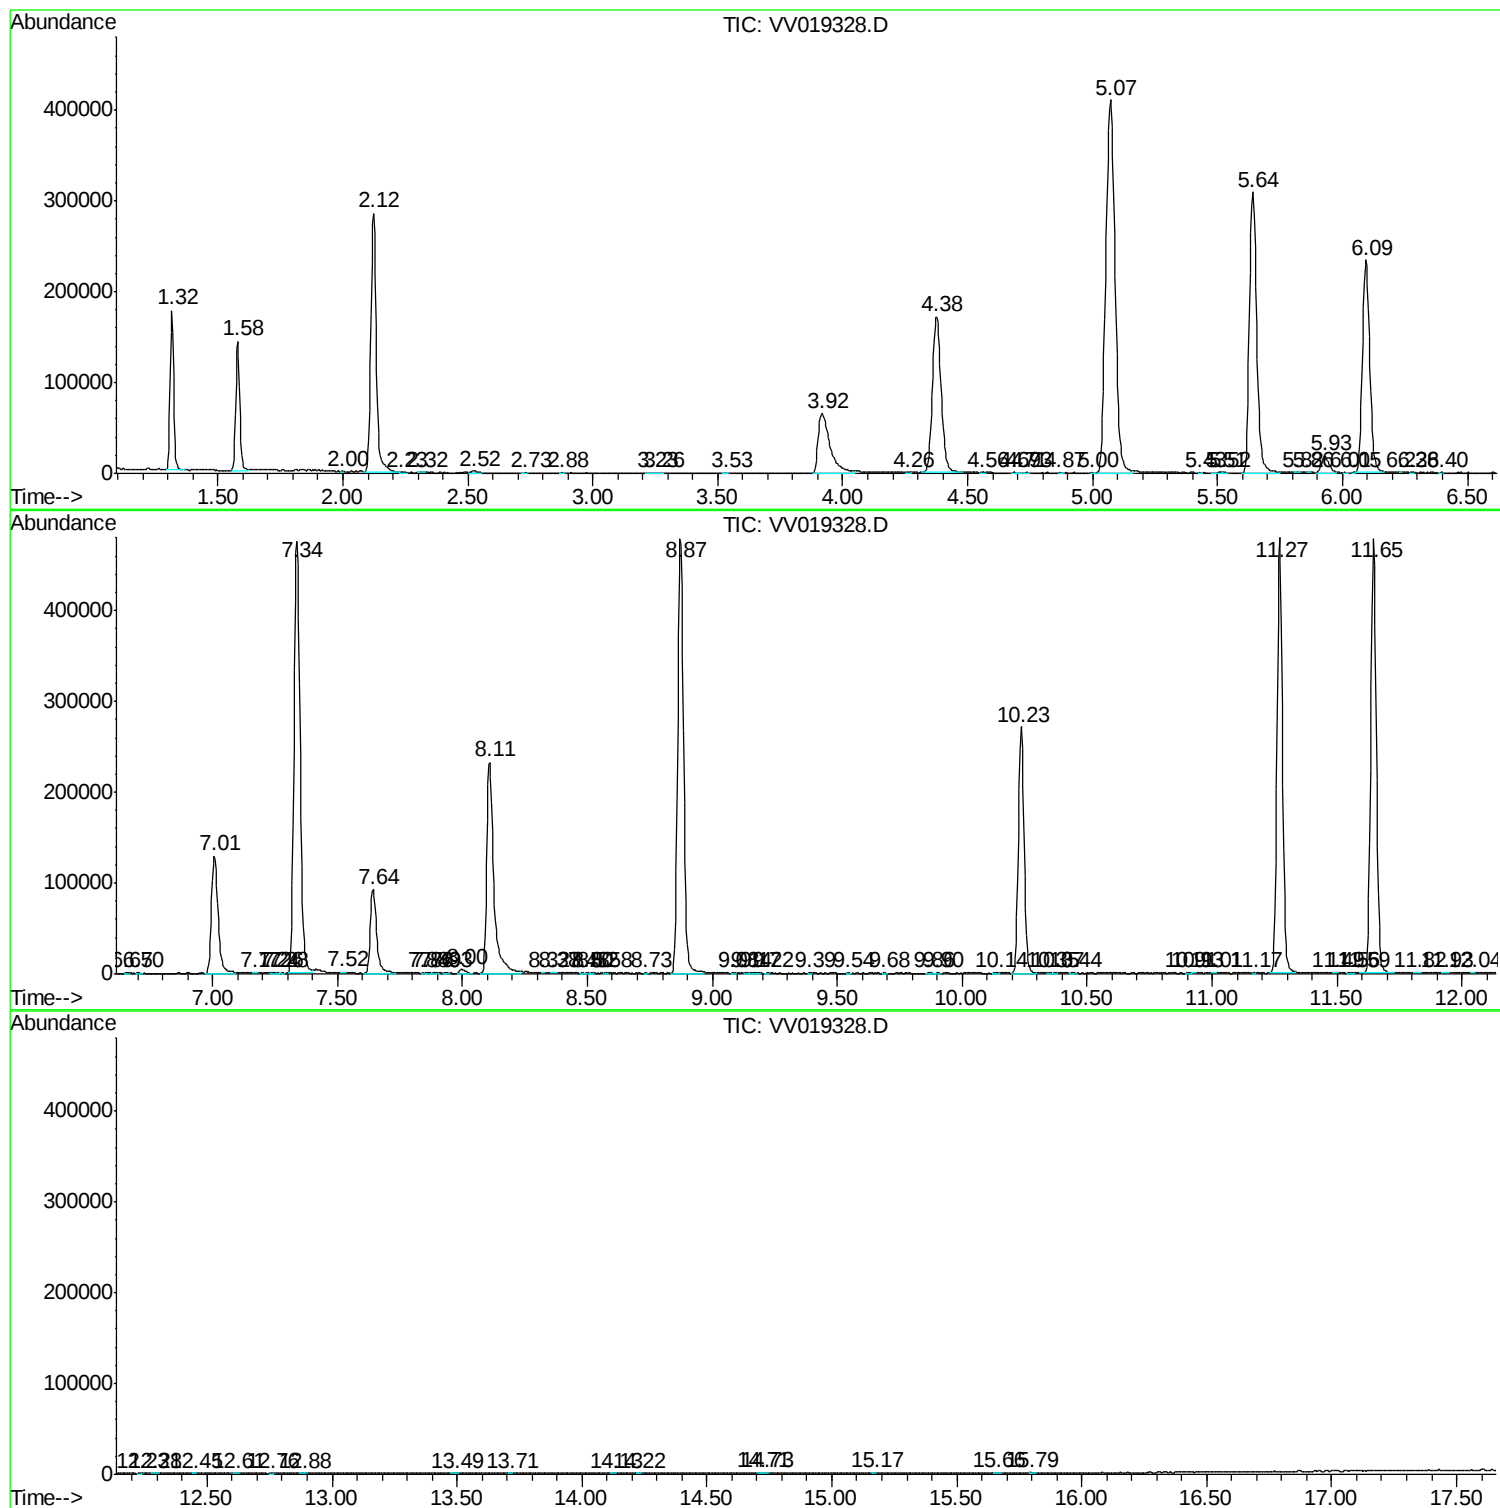

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV111020\
Data File : VV019328.D
Acq On : 10 Nov 2020 17:05
Operator : SY/MD
Sample : VIBLK95
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK95

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV111020\
Data File : VV019328.D
Acq On : 10 Nov 2020 17:05
Operator : SY/MD
Sample : VIBLK95
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK95

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc