


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV111020\
 Data File : VV019311.D
 Acq On : 10 Nov 2020 08:59
 Operator : SY/MD
 Sample : BFB91
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB91

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102920WMA.M
 Title : VOC Analysis
 Last Update : Wed Nov 11 02:14:49 2020

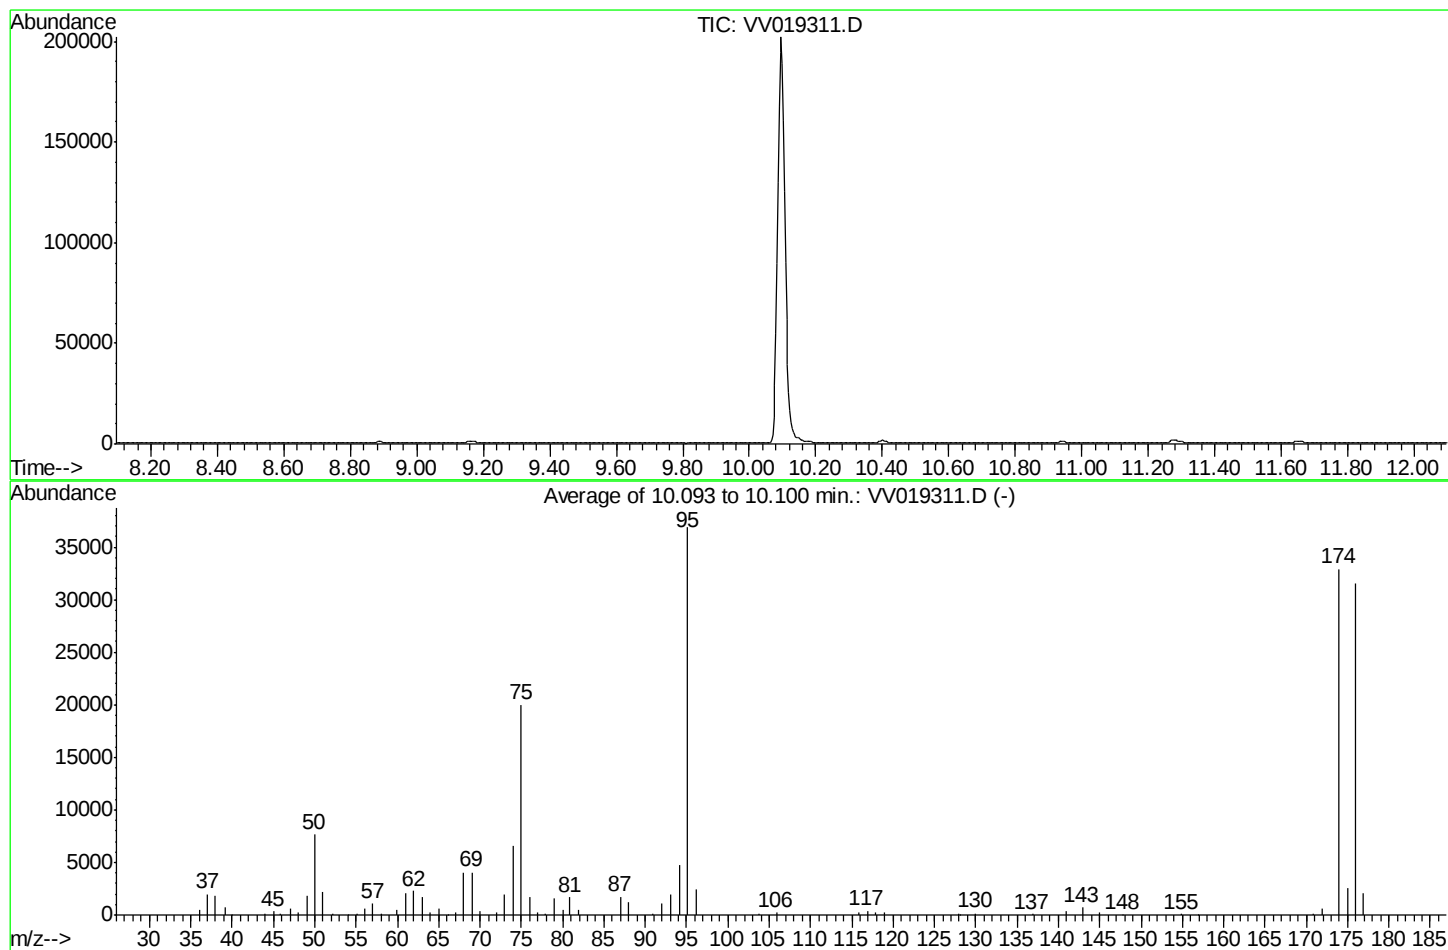

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	7662	PASS
75	95	30	80	54.2	20000	PASS
95	95	100	100	100.0	36874	PASS
96	95	5	9	6.5	2398	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	89.2	32888	PASS
175	174	5	9	7.8	2560	PASS
176	174	95	101	95.8	31520	PASS
177	176	5	9	6.6	2085	PASS

m/z	Abundance
36.00	440.0
37.00	2087.0
38.00	1957.0
39.10	808.0
40.00	143.0
44.00	674.0
45.10	322.0
47.00	633.0
48.00	273.0
49.00	1761.0
50.00	7887.0
51.00	2281.0
52.10	112.0
55.10	127.0
56.00	584.0
57.00	1092.0
58.00	103.0
59.90	427.0
61.00	2129.0
62.00	2263.0
63.00	1644.0
64.00	275.0
65.10	604.0
66.10	126.0
67.00	229.0
68.00	3868.0
69.00	4242.0
70.00	376.0
72.00	229.0
73.00	1821.0
74.00	6806.0
75.00	20400.0
76.10	1792.0
77.00	263.0
77.90	202.0
78.90	1558.0
80.00	480.0
80.90	1690.0
82.00	424.0
87.00	1735.0
88.00	1188.0
90.90	208.0
92.00	1138.0
93.00	1878.0
94.10	4803.0
95.10	37032.0
96.10	2500.0
103.80	148.0
105.90	231.0
115.80	193.0
116.90	378.0
117.80	212.0
118.90	261.0
127.90	149.0
130.00	172.0
136.90	109.0
140.90	377.0
142.90	647.0
145.00	208.0
147.80	109.0
170.90	106.0
172.00	593.0
174.00	31776.0
175.00	2614.0
176.00	30880.0
177.00	2041.0

Instrument :
MSVOA_V
ClientSampleId :
BFB91

m/z	Abundance
36.00	459.0
37.00	2050.0
38.00	1982.0
39.10	765.0
40.00	144.0
44.00	652.0
45.00	339.0
45.80	137.0
47.00	590.0
48.00	241.0
49.00	1863.0
50.00	7934.0
51.00	2242.0
52.10	151.0
55.10	164.0
56.00	626.0
57.00	1081.0
58.00	130.0
59.90	450.0
61.00	2149.0
62.00	2400.0
63.00	1847.0
63.90	279.0
65.10	621.0
67.10	209.0
68.00	4150.0
69.00	4135.0
70.00	301.0
72.00	205.0
73.00	1988.0
74.00	6824.0
75.00	20624.0
76.00	1759.0
77.00	261.0
77.90	190.0
78.90	1640.0
80.00	488.0
80.90	1701.0
81.90	472.0
87.00	1866.0
88.00	1308.0
90.90	191.0
92.00	1158.0
93.00	1974.0
94.10	5023.0
95.10	38216.0
96.10	2419.0
103.80	162.0
105.90	226.0
115.90	210.0
116.90	421.0
117.80	250.0
118.90	281.0
127.90	132.0
130.00	168.0
136.90	130.0
140.90	412.0
142.90	731.0
144.90	201.0
155.00	123.0
156.90	104.0
170.90	119.0
171.90	647.0
174.00	34040.0
175.00	2646.0
176.00	32672.0
177.00	2142.0

Instrument :
MSVOA_V
ClientSampleId :
BFB91

m/z	Abundance
36.00	427.0
37.00	1847.0
38.00	1733.0
39.10	718.0
40.00	147.0
44.00	628.0
44.90	363.0
45.80	165.0
47.00	515.0
47.90	176.0
49.00	1726.0
50.00	7166.0
51.00	2089.0
52.10	159.0
54.00	102.0
55.10	153.0
56.00	650.0
57.00	958.0
58.00	117.0
60.00	442.0
61.00	1949.0
62.00	2164.0
63.00	1774.0
63.90	267.0
65.00	538.0
67.10	151.0
68.00	3913.0
69.00	3703.0
70.10	262.0
72.00	171.0
73.00	1879.0
74.10	6167.0
75.00	18976.0
76.00	1528.0
77.00	230.0
79.00	1578.0
80.00	455.0
80.90	1578.0
81.90	474.0
87.00	1614.0
88.00	1337.0
90.80	153.0
92.00	1052.0
93.00	1878.0
94.10	4610.0
95.10	35376.0
96.10	2275.0
103.80	194.0
105.90	210.0
115.90	177.0
116.90	411.0
117.80	277.0
118.90	273.0
128.10	141.0
130.00	124.0
136.90	121.0
140.90	376.0
142.90	691.0
144.80	224.0
154.90	130.0
170.90	126.0
171.90	649.0
174.00	32848.0
175.00	2421.0
176.00	31008.0
176.90	2073.0

Instrument :
MSVOA_V
ClientSampleId :
BFB91

Scan 2789 (10.058 min): VV019311.D
BFB91

m/z	Abundance
40.00	111.0
44.10	505.0

Instrument :
MSVOA_V
ClientSampleId :
BFB91