

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
 Data File : VV023371.D
 Acq On : 11 Nov 2021 08:01
 Operator : SY/MD
 Sample : VV1110WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK248

Quant Time: Nov 11 08:19:51 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 11 08:19:32 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	120864	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	120816	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	58159	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	36633	4.838	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	96.800%	
7) Chloroethane-d5	1.568	69	30139	4.884	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	97.600%	
11) 1,1-Dichloroethene-d2	2.111	63	51619	3.642	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	72.800%	
20) 2-Butanone-d5	3.889	46	70919	54.366	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	108.740%	
24) Chloroform-d	4.352	84	71386	4.424	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	88.400%	
26) 1,2-Dichloroethane-d4	5.034	65	32623	4.496	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	90.000%	
32) Benzene-d6	5.053	84	141208	4.555	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.200%	
36) 1,2-Dichloropropane-d6	6.072	67	41073	4.501	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	90.000%	
41) Toluene-d8	7.317	98	122635	4.222	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	84.400%	
43) trans-1,3-Dichloroprop...	7.625	79	14478	4.184	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	83.600%	
46) 2-Hexanone-d5	8.091	63	51141	40.171	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	80.340%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	27282	4.157	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	83.200%	
66) 1,2-Dichlorobenzene-d4	11.625	152	46037	4.754	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	95.000%	
Target Compounds						Qvalue
34) Trichloroethene	5.921	95	1661	0.185	ug/L	# 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023371.D
Acq On : 11 Nov 2021 08:01
Operator : SY/MD
Sample : VV1110WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK248


Quant Time: Nov 11 08:19:51 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 11 08:19:32 2021
Response via : Initial Calibration

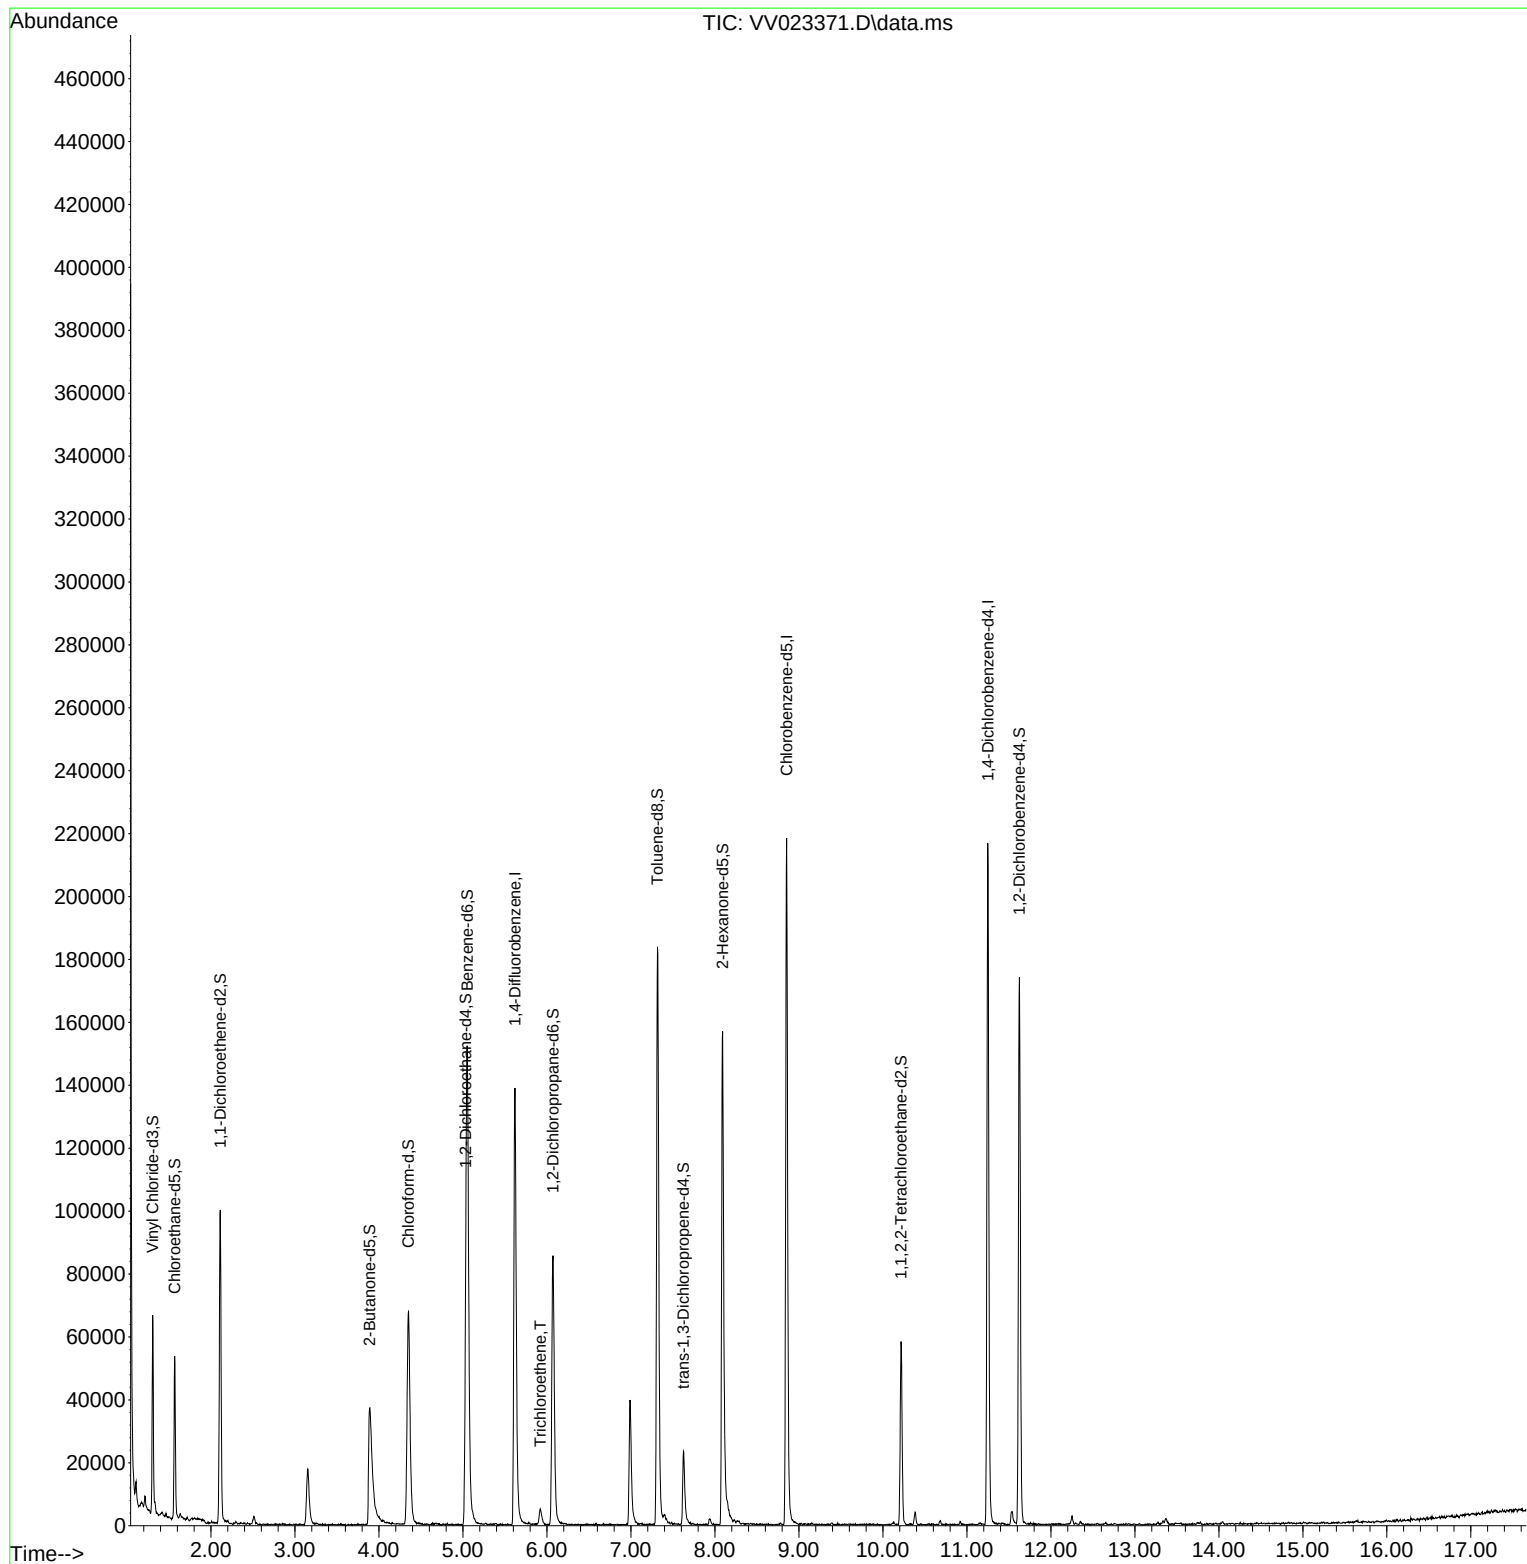

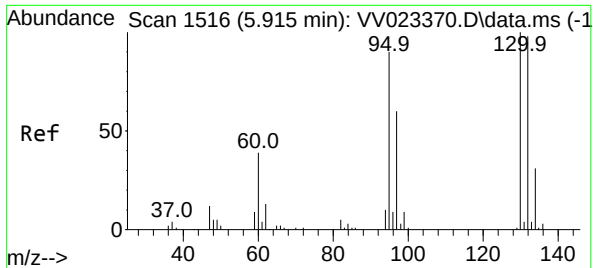

#34
 Trichloroethene
 Concen: 0.185 ug/L
 RT: 5.921 min Scan# 11
 Delta R.T. 0.006 min
 Lab File: VV023371.D
 Acq: 11 Nov 2021 08:01

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK248

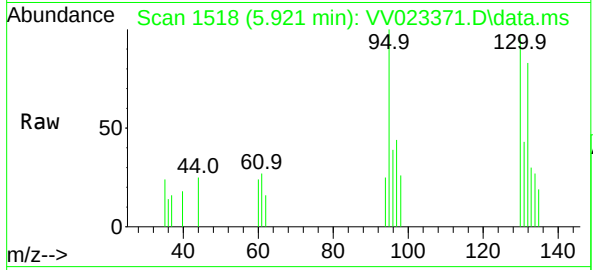

Tgt Ion: 95 Resp: 1661

Ion	Ratio	Lower	Upper
95	100		
97	43.9	45.0	83.6#
132	83.3	69.7	129.4
130	95.6	73.7	136.9

