

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111021\
 Data File : VW023372.D
 Acq On : 11 Nov 2021 08:47
 Operator : SY/MD
 Sample : M4558-11DL 40X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB873DL

Quant Time: Nov 12 00:27:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 11 08:19:32 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	130884	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	127064	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	62864	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	36628	4.467	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	89.400%	
7) Chloroethane-d5	1.568	69	30681	4.591	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	91.800%	
11) 1,1-Dichloroethene-d2	2.108	63	52685	3.432	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	68.600%	
20) 2-Butanone-d5	3.886	46	673			

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023372.D
Acq On : 11 Nov 2021 08:47
Operator : SY/MD
Sample : M4558-11DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB873DL

Quant Time: Nov 12 00:27:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 11 08:19:32 2021
Response via : Initial Calibration

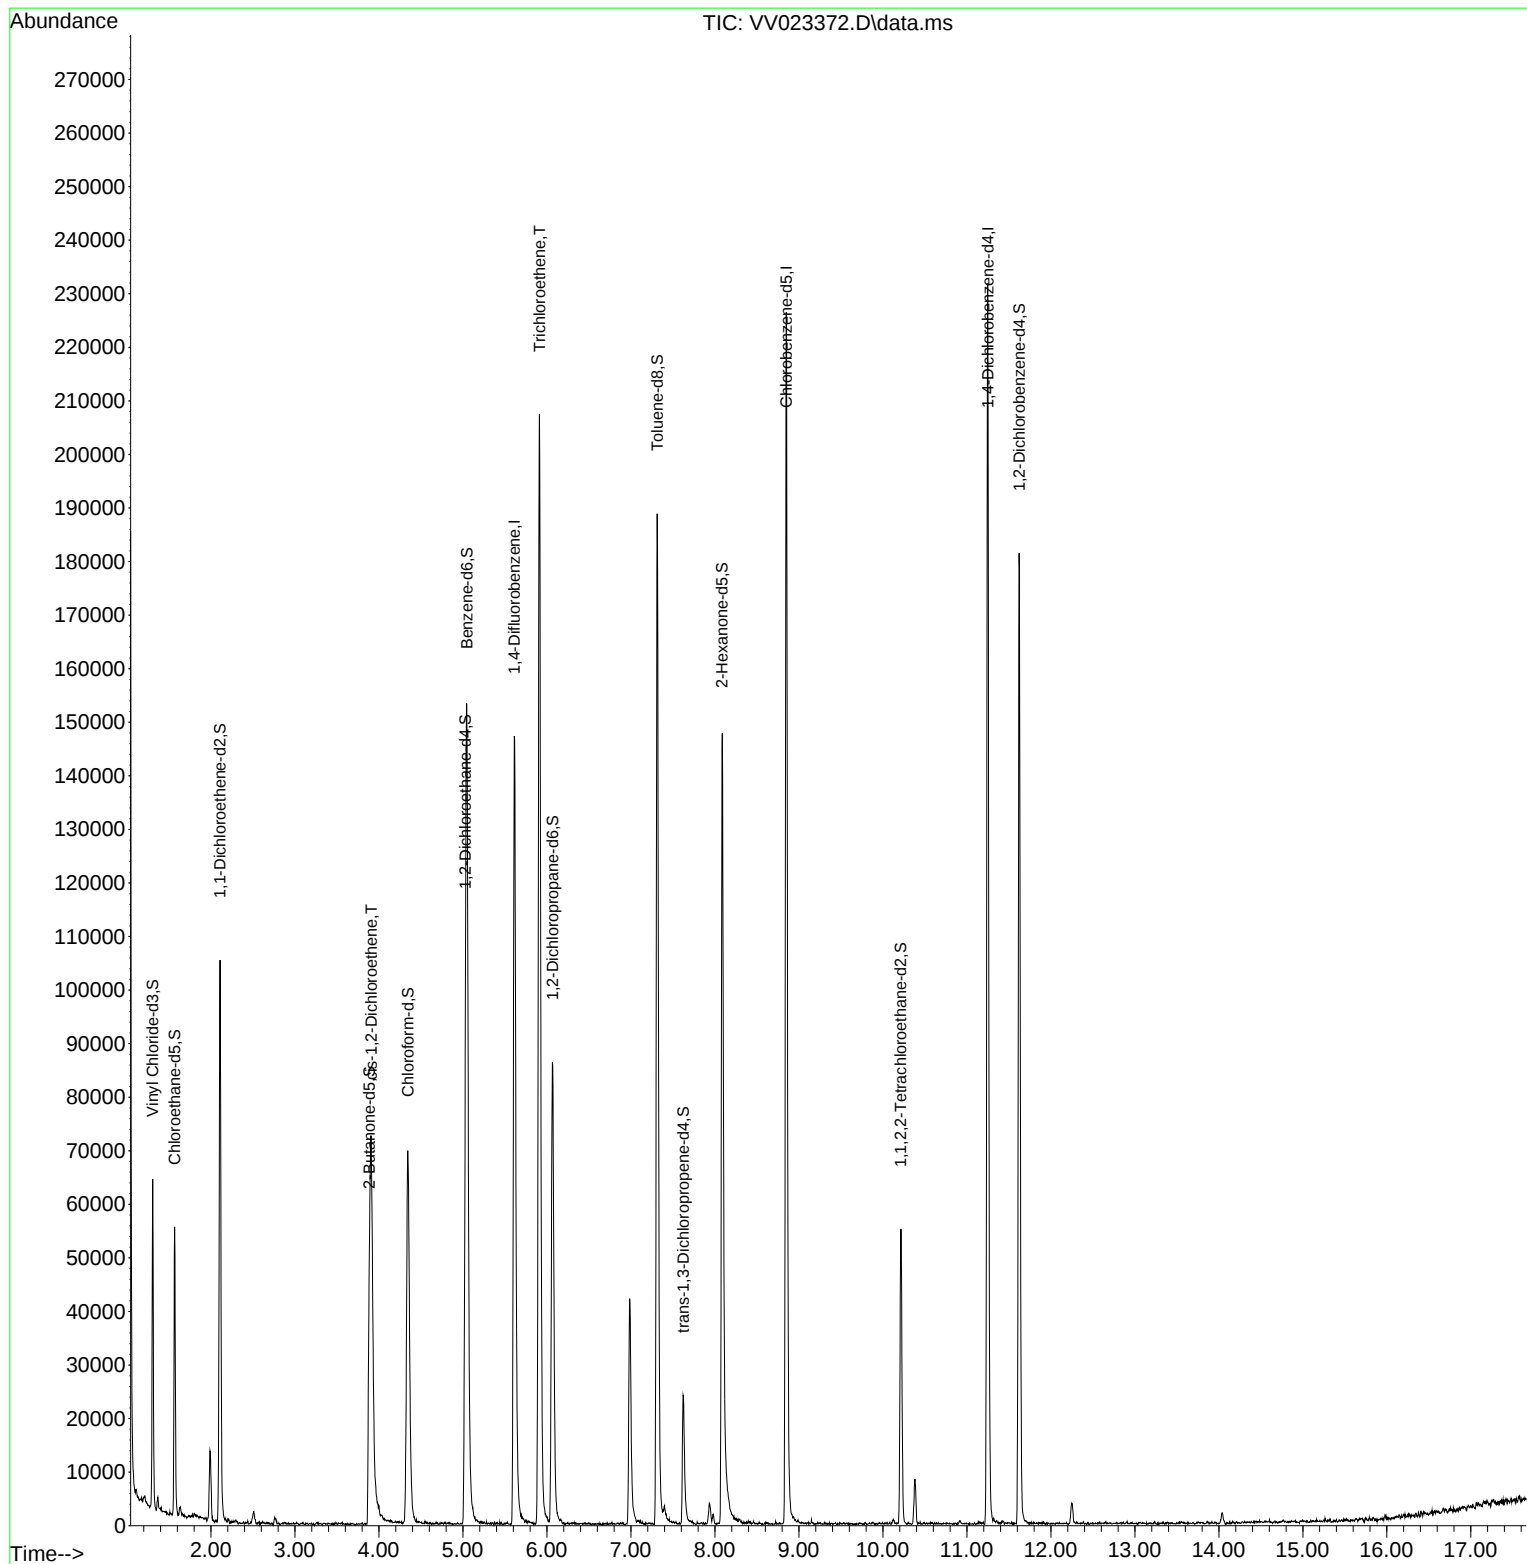

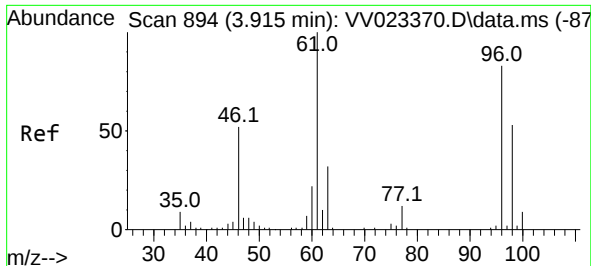

#22

cis-1,2-Dichloroethene

Concen: 3.120 ug/L

RT: 3.908 min Scan# 894

Delta R.T. -0.007 min

Lab File: VV023372.D

Acq: 11 Nov 2021 08:47

Instrument :

MSVOA_V

ClientSampleId :

GB873DL

Tgt Ion: 96 Resp: 28813

Ion Ratio Lower Upper

96 100

61 125.0 92.3 171.3

68 0.0 0.4 0.8#

