

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111021\
 Data File : VW023373.D
 Acq On : 11 Nov 2021 09:10
 Operator : SY/MD
 Sample : M4558-13DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB875DL

Quant Time: Nov 12 00:27:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 11 08:19:32 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	122667	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	121208	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	59147	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	36529	4.754	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	95.000%	
7) Chloroethane-d5	1.568	69	29652	4.734	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	94.600%	
11) 1,1-Dichloroethene-d2	2.108	63	51440	3.576	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	71.600%	
20) 2-Butanone-d5	3.902	46	65040	49.127	ug/L	0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	98.260%	
24) Chloroform-d	4.352	84	70558	4.308	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	86.200%	
26) 1,2-Dichloroethane-d4	5.037	65	34149	4.637	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	92.800%	
32) Benzene-d6	5.053	84	137122	4.409	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	88.200%	
36) 1,2-Dichloropropane-d6	6.072	67	41754	4.561	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	91.200%	
41) Toluene-d8	7.317	98	125110	4.293	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.800%	
43) trans-1,3-Dichloroprop...	7.625	79	14817	4.268	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	85.400%	
46) 2-Hexanone-d5	8.091	63	51791	40.550	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	81.100%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	26942	4.092	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	81.800%	
66) 1,2-Dichlorobenzene-d4	11.625	152	47780	4.851	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	97.000%	
Target Compounds						
22) cis-1,2-Dichloroethene	3.915	96	9362	1.082	ug/L	Qvalue # 93
34) Trichloroethene	5.915	95	73666	8.177	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023373.D
Acq On : 11 Nov 2021 09:10
Operator : SY/MD
Sample : M4558-13DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB875DL

Quant Time: Nov 12 00:27:26 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 11 08:19:32 2021
Response via : Initial Calibration

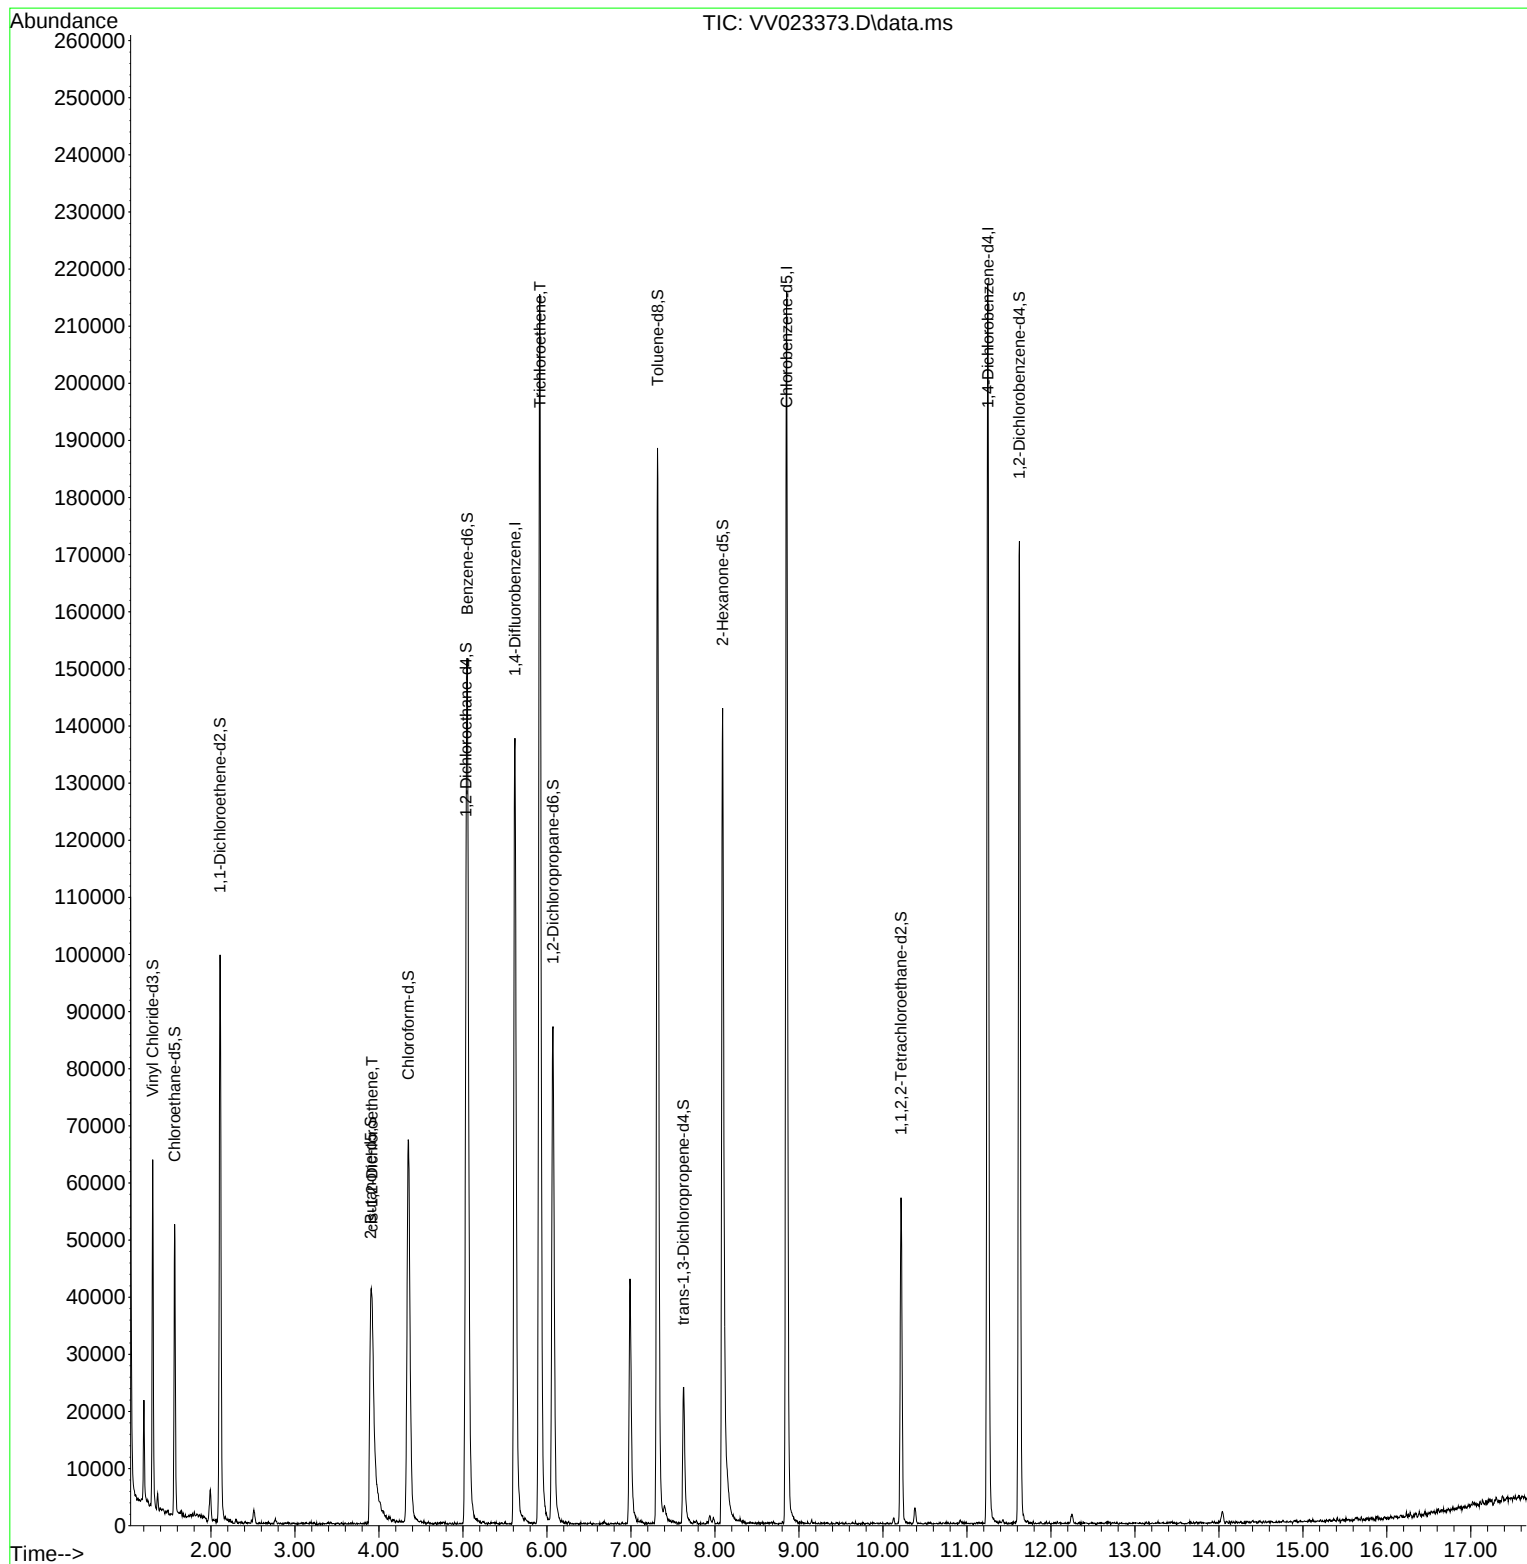

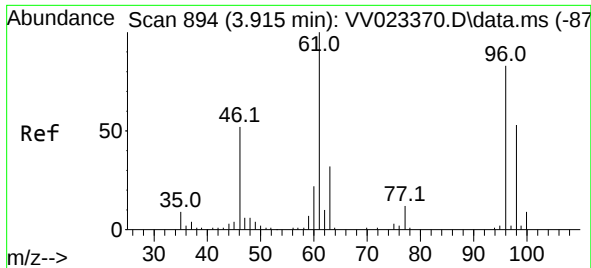

#22

cis-1,2-Dichloroethene

Concen: 1.082 ug/L

RT: 3.915 min Scan# 894

Delta R.T. -0.000 min

Lab File: VV023373.D

Acq: 11 Nov 2021 09:10

Instrument :

MSVOA_V

ClientSampleId :

GB875DL





Tgt Ion: 96 Resp: 9362

Ion Ratio Lower Upper

96 100

61 123.7 92.3 171.3

68 0.0 0.4 0.8#

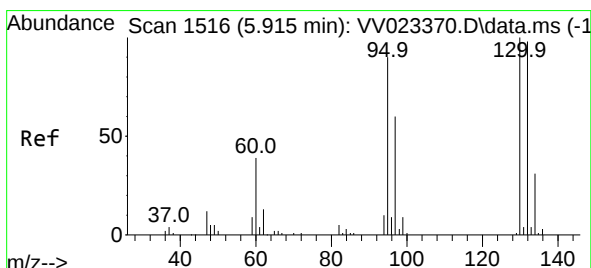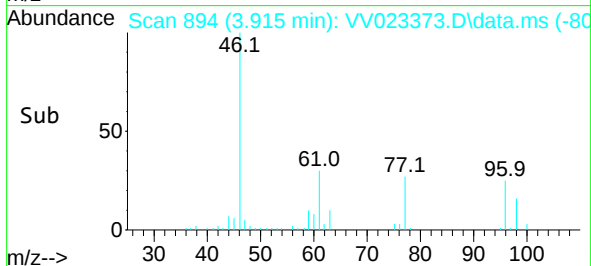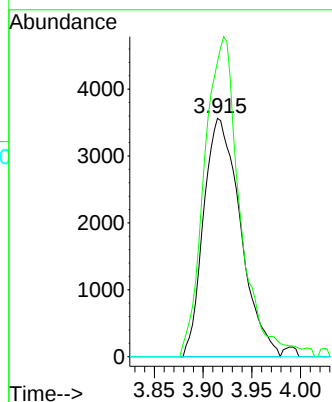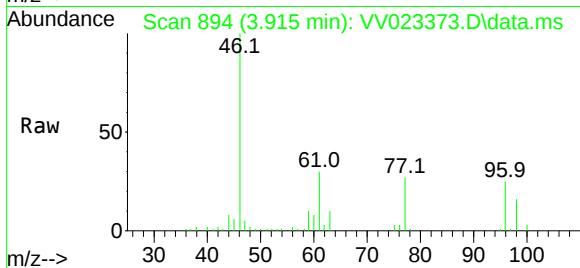

#34

Trichloroethene

Concen: 8.177 ug/L

RT: 5.915 min Scan# 1516

Delta R.T. -0.000 min

Lab File: VV023373.D

Acq: 11 Nov 2021 09:10

Tgt Ion: 95 Resp: 73666

Ion Ratio Lower Upper

95 100

97 64.3 45.0 83.6

132 102.6 69.7 129.4

130 107.9 73.7 136.9

