

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111021\
 Data File : VW023402.D
 Acq On : 11 Nov 2021 20:59
 Operator : SY/MD
 Sample : M4542-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGGF7

Quant Time: Nov 12 02:09:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 12 02:02:21 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	119588	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	115560	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	53358	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	31143	4.157	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.200%
7) Chloroethane-d5	1.568	69	25971	4.253	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.000%
11) 1,1-Dichloroethene-d2	2.108	63	44358	3.163	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.200%
20) 2-Butanone-d5	3.892	46	72361	56.064	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.120%
24) Chloroform-d	4.349	84	66817	4.185	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.600%
26) 1,2-Dichloroethane-d4	5.034	65	33115	4.612	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.200%
32) Benzene-d6	5.050	84	131768	4.444	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.800%
36) 1,2-Dichloropropane-d6	6.069	67	39266	4.499	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.000%
41) Toluene-d8	7.317	98	113569	4.087	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.800%
43) trans-1,3-Dichloroprop...	7.625	79	13959	4.218	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.400%
46) 2-Hexanone-d5	8.092	63	52289	42.941	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.880%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	25661	4.088	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	81.800%
66) 1,2-Dichlorobenzene-d4	11.625	152	44815	5.044	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.800%
Target Compounds					Qvalue	
13) Acetone	2.182	43	8136	10.316	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023402.D
Acq On : 11 Nov 2021 20:59
Operator : SY/MD
Sample : M4542-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGGF7

Quant Time: Nov 12 02:09:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 12 02:02:21 2021
Response via : Initial Calibration

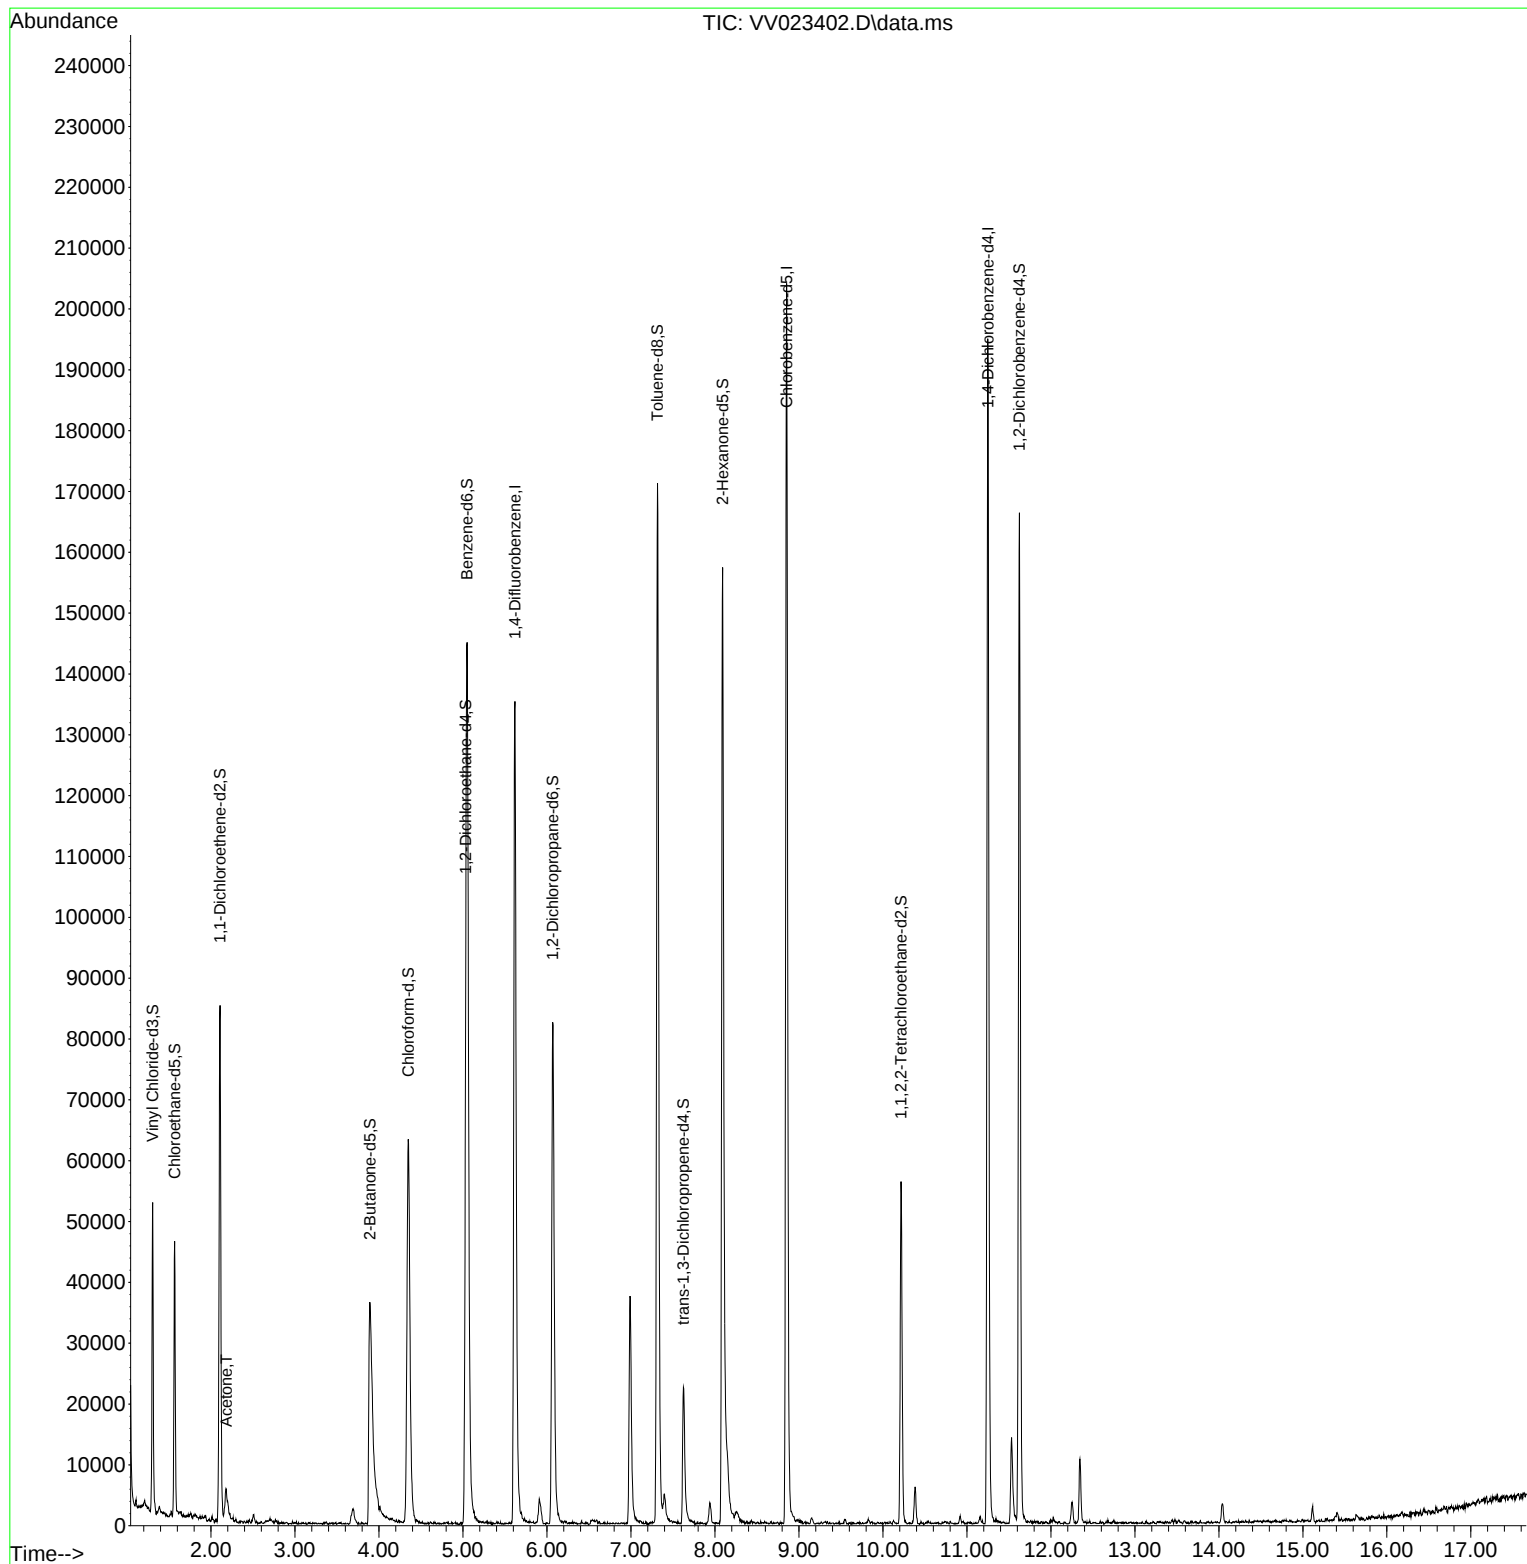

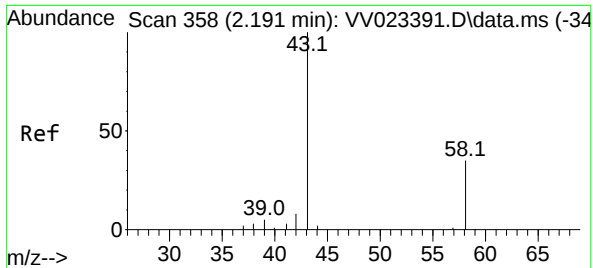

#13
 Acetone
 Concen: 10.316 ug/L
 RT: 2.182 min Scan# 31
 Delta R.T. -0.009 min
 Lab File: VV023402.D
 Acq: 11 Nov 2021 20:59

Instrument :
 MSVOA_V
 ClientSampleId :
 BGGF7

Tgt Ion: 43 Resp: 8136
 Ion Ratio Lower Upper
 43 100
 58 29.8 0.0 55.4

