

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
 Data File : VV023355.D
 Acq On : 11 Nov 2021 01:00
 Operator : SY/MD
 Sample : M4558-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB876

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023355.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.992	286	296	308	rBV	79732	122424	1.79%	1.118%
2	2.111	323	333	346	rVB	72557	104676	1.53%	0.956%
3	3.911	875	893	925	rBV2	338176	922099	13.50%	8.421%
4	4.352	1013	1030	1051	rBV2	69037	173872	2.55%	1.588%
5	5.050	1231	1247	1275	rBV3	150880	381519	5.59%	3.484%
6	5.619	1412	1424	1445	rBV	153274	312253	4.57%	2.852%
7	5.915	1501	1516	1551	rBV	3637220	6828826	100.00%	62.365%
8	6.072	1554	1565	1592	rVB2	92034	195180	2.86%	1.783%
9	6.992	1840	1851	1876	rBV	37183	73342	1.07%	0.670%
10	7.320	1940	1953	1972	rBV	165869	293737	4.30%	2.683%
11	8.091	2182	2193	2220	rBV	212988	395881	5.80%	3.615%
12	8.853	2419	2430	2446	rBV	239484	385707	5.65%	3.523%
13	10.217	2840	2854	2870	rBV	71251	112972	1.65%	1.032%
14	11.249	3164	3175	3202	rBV	235250	362151	5.30%	3.307%
15	11.625	3281	3292	3313	rBV	179726	285139	4.18%	2.604%




Sum of corrected areas: 10949778

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023355.D
Acq On : 11 Nov 2021 01:00
Operator : SY/MD
Sample : M4558-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB876

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

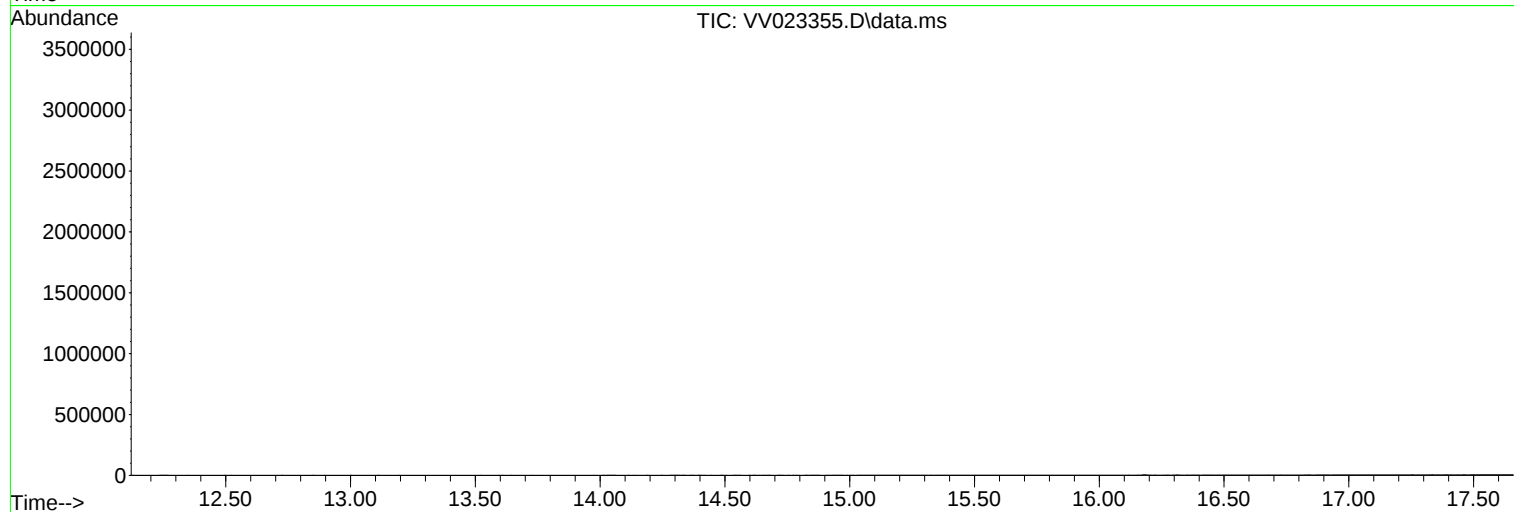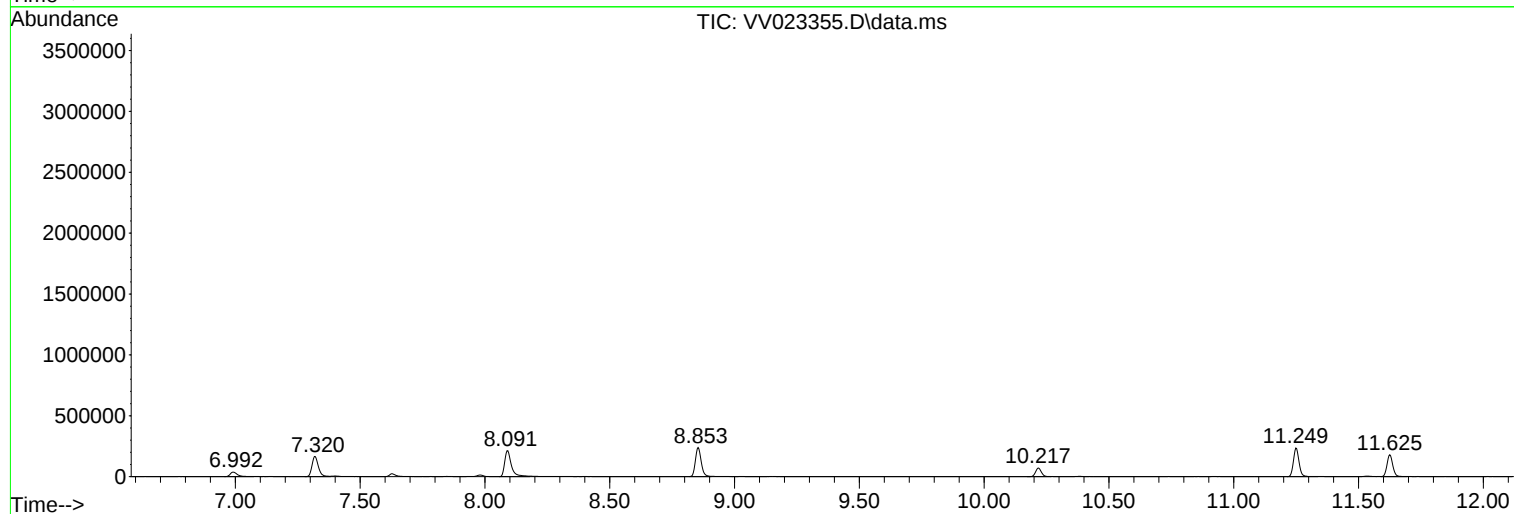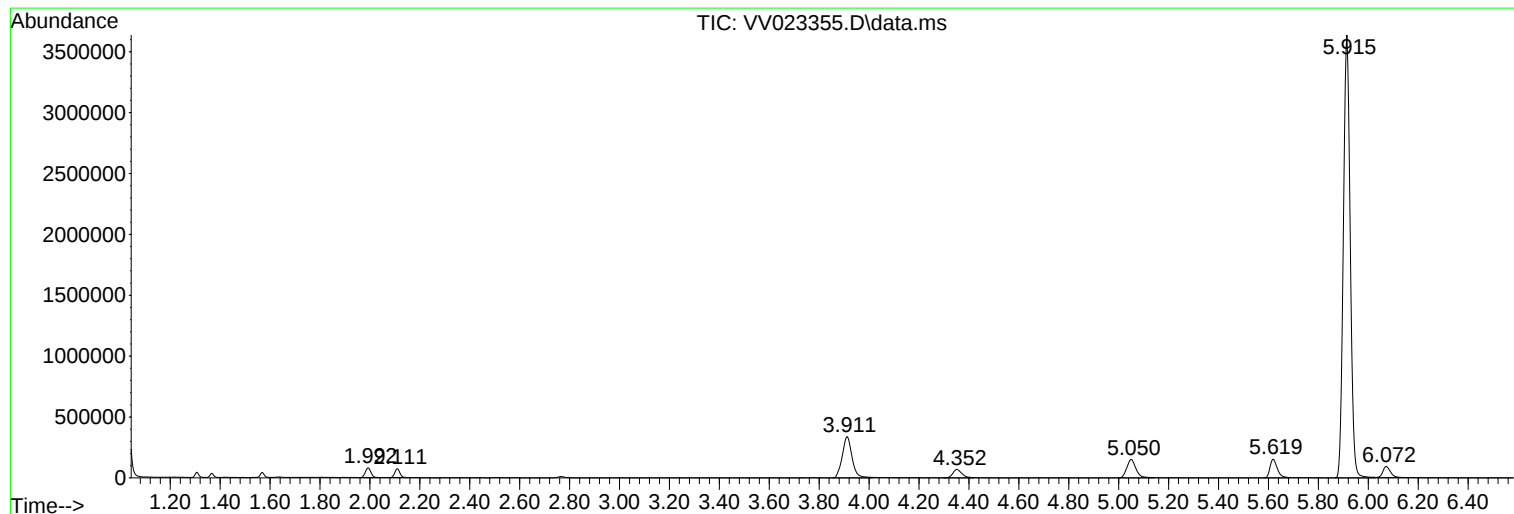

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023355.D
Acq On : 11 Nov 2021 01:00
Operator : SY/MD
Sample : M4558-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB876









Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethane, 2,2-dichloro-1,1,1-... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.992	1.96 ug/L	122424	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethane, 2,2-dichloro-1,1,1-trifl...	152	C2HCl2F3	000306-83-2	94
2			Ethane, 2,2-dichloro-1,1,1-trifl...	152	C2HCl2F3	000306-83-2	93
3			Ethane, 2,2-dichloro-1,1,1-trifl...	152	C2HCl2F3	000306-83-2	90
4			Ethane, 1,2,2-trichloro-1,1-difl...	168	C2HCl3F2	000354-21-2	59
5			Methane, dichloronitro-	129	CHCl2NO2	007119-89-3	59

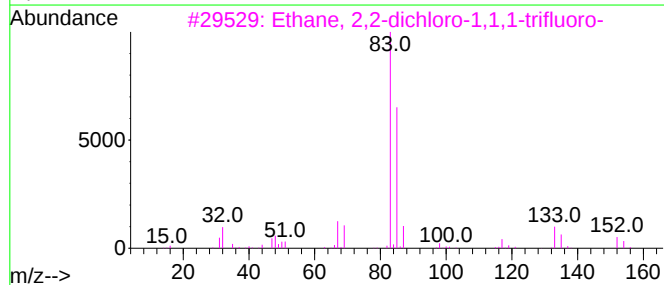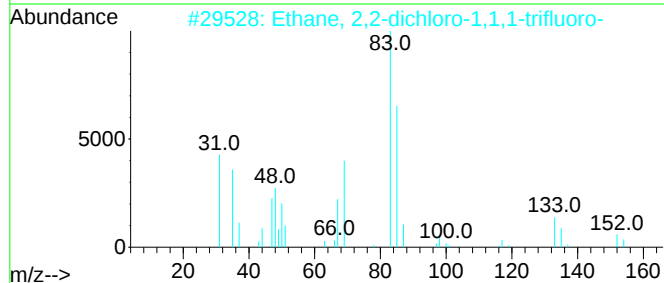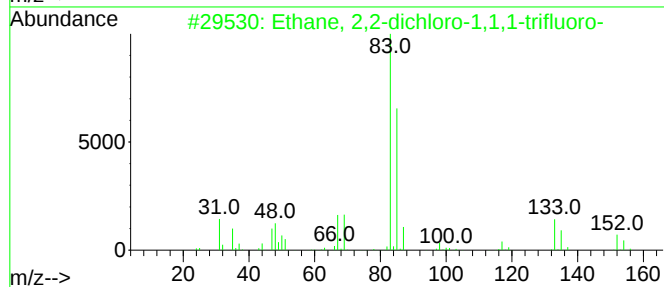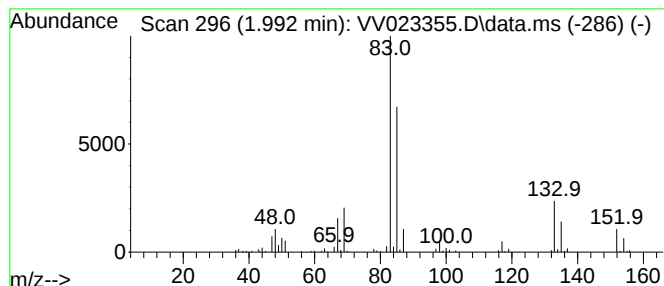

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023355.D
Acq On : 11 Nov 2021 01:00
Operator : SY/MD
Sample : M4558-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB876

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethane, 2,2-dic...	1.992	2.0	ug/L	122424	1	5.619	312253	5.0