

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
 Data File : VV023367.D
 Acq On : 11 Nov 2021 05:41
 Operator : SY/MD
 Sample : M4542-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGGF6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023367.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.243	57	63	71	rVV	12704	14666	3.76%	0.414%
2	1.307	75	83	95	rVB	42214	45170	11.59%	1.275%
3	1.568	157	164	172	rBV	42752	47322	12.14%	1.335%
4	2.015	292	303	312	rBV4	3901	6444	1.65%	0.182%
5	2.111	323	333	346	rBV	73962	109492	28.09%	3.090%
6	2.175	346	353	370	rVB	8151	17712	4.54%	0.500%
7	2.327	386	400	402	rBV8	3705	6548	1.68%	0.185%
8	3.886	873	885	918	rBV	54067	166097	42.62%	4.687%
9	4.352	1013	1030	1055	rBV	70052	176124	45.19%	4.970%
10	5.050	1231	1247	1277	rBV3	151145	385465	98.91%	10.878%
11	5.619	1412	1424	1452	rBV2	152783	314735	80.76%	8.882%
12	5.921	1505	1518	1537	rBV7	12519	30563	7.84%	0.862%
13	6.072	1551	1565	1585	rBV2	89044	187152	48.02%	5.281%
14	6.577	1712	1722	1731	rVB8	3021	5943	1.52%	0.168%
15	6.989	1836	1850	1865	rBV	41608	77011	19.76%	2.173%
16	7.137	1886	1896	1912	rVB7	4539	8933	2.29%	0.252%
17	7.317	1940	1952	1969	rBV	170040	301406	77.34%	8.506%
18	7.400	1974	1978	1987	rVB6	3204	4396	1.13%	0.124%
19	7.625	2039	2048	2066	rBV	24655	44938	11.53%	1.268%
20	8.088	2181	2192	2228	rBV	197921	377713	96.92%	10.659%
21	8.252	2234	2243	2258	rVB5	5586	11145	2.86%	0.315%
22	8.854	2419	2430	2453	rBV	237755	389727	100.00%	10.998%
23	10.217	2843	2854	2871	rBV2	62712	103409	26.53%	2.918%
24	10.387	2897	2907	2915	rVB5	2980	4789	1.23%	0.135%
25	11.249	3164	3175	3193	rBV	242524	376729	96.66%	10.631%
26	11.532	3255	3263	3277	rBV3	7077	13308	3.41%	0.376%
27	11.625	3281	3292	3308	rVV	188465	297194	76.26%	8.387%
28	12.345	3508	3516	3526	rBV4	12642	19488	5.00%	0.550%




Sum of corrected areas: 3543619

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023367.D
Acq On : 11 Nov 2021 05:41
Operator : SY/MD
Sample : M4542-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGGF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

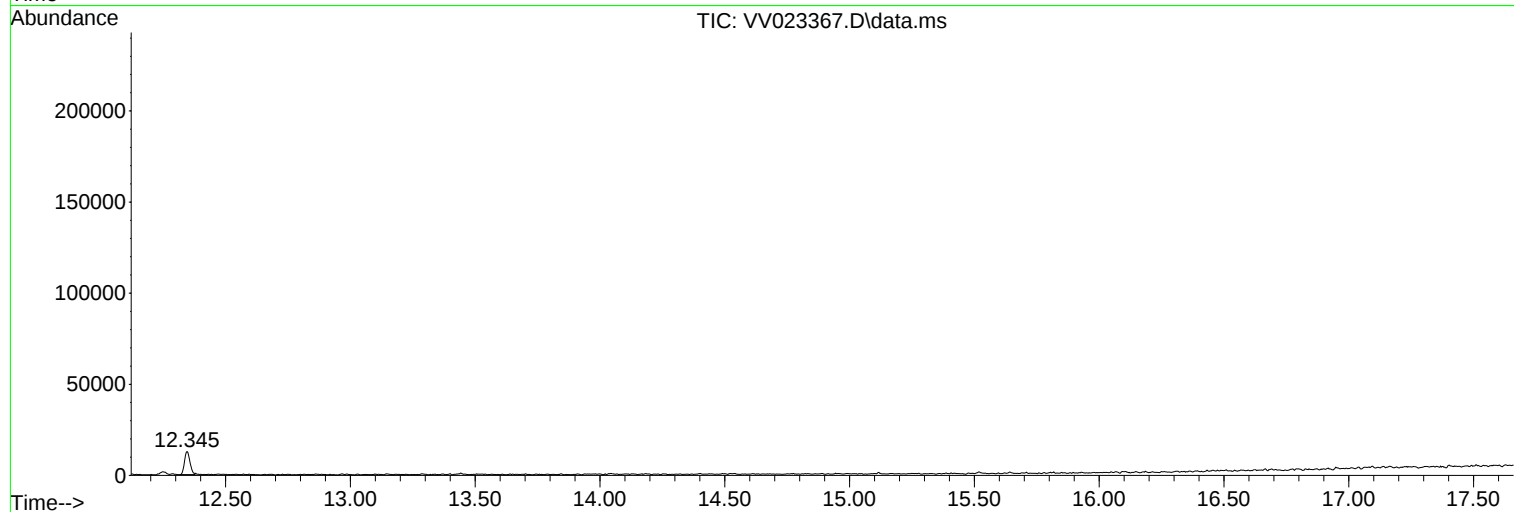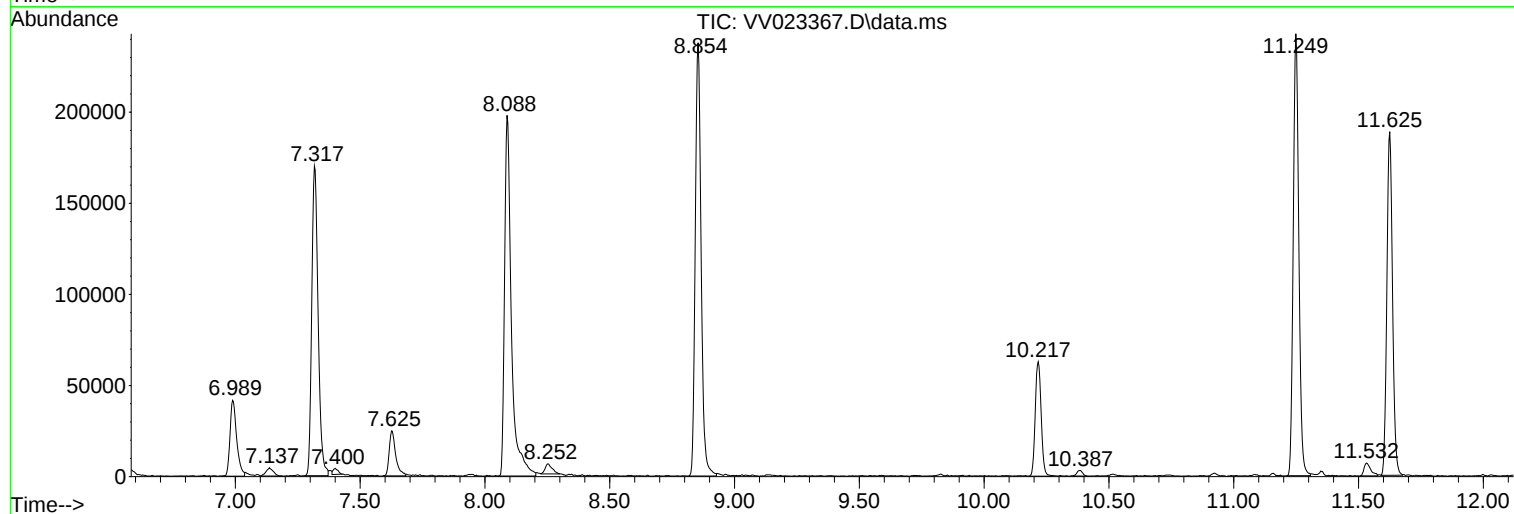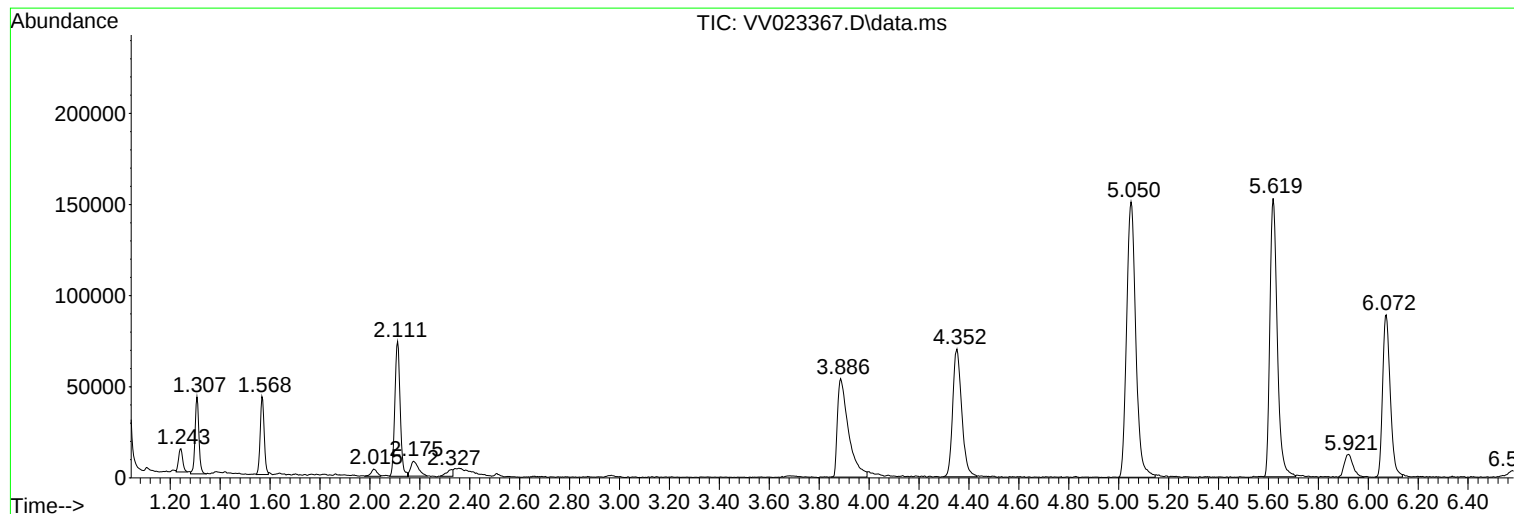

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023367.D
Acq On : 11 Nov 2021 05:41
Operator : SY/MD
Sample : M4542-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGGF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023367.D
Acq On : 11 Nov 2021 05:41
Operator : SY/MD
Sample : M4542-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGGF6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc