

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
 Data File : VV023372.D
 Acq On : 11 Nov 2021 08:47
 Operator : SY/MD
 Sample : M4558-11DL 40X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB873DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023372.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	61861	63538	15.42%	1.645%
2	1.568	156	164	175	rVB	53682	59885	14.53%	1.551%
3	1.989	283	295	308	rBV2	13141	19861	4.82%	0.514%
4	2.108	321	332	350	rBV	104951	150996	36.64%	3.910%
5	3.905	876	891	918	rBV4	72533	234902	57.01%	6.083%
6	4.342	1011	1027	1058	rBV	69486	175093	42.49%	4.534%
7	5.043	1229	1245	1274	rBV2	153187	387909	94.14%	10.045%
8	5.612	1411	1422	1450	rBV	147056	300213	72.86%	7.774%
9	5.911	1500	1515	1536	rBV	207230	412068	100.00%	10.671%
10	6.066	1552	1563	1590	rBV2	85678	179221	43.49%	4.641%
11	6.985	1839	1849	1874	rBV2	42077	81584	19.80%	2.113%
12	7.313	1940	1951	1971	rBV	188666	329882	80.06%	8.543%
13	7.622	2035	2047	2066	rBV2	24121	45682	11.09%	1.183%
14	7.934	2134	2144	2153	rBV3	3962	7125	1.73%	0.185%
15	8.088	2181	2192	2234	rBV	147572	286191	69.45%	7.411%
16	8.850	2414	2429	2453	rBV	226242	373068	90.54%	9.661%
17	10.214	2842	2853	2873	rVB2	55049	89905	21.82%	2.328%
18	10.381	2892	2905	2915	rBV2	8489	13856	3.36%	0.359%
19	11.249	3163	3175	3194	rBV	231734	357356	86.72%	9.254%
20	11.622	3280	3291	3311	rBV	181213	285437	69.27%	7.392%
21	12.249	3473	3486	3501	rBV2	4050	7875	1.91%	0.204%




Sum of corrected areas: 3861647

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023372.D
Acq On : 11 Nov 2021 08:47
Operator : SY/MD
Sample : M4558-11DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB873DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

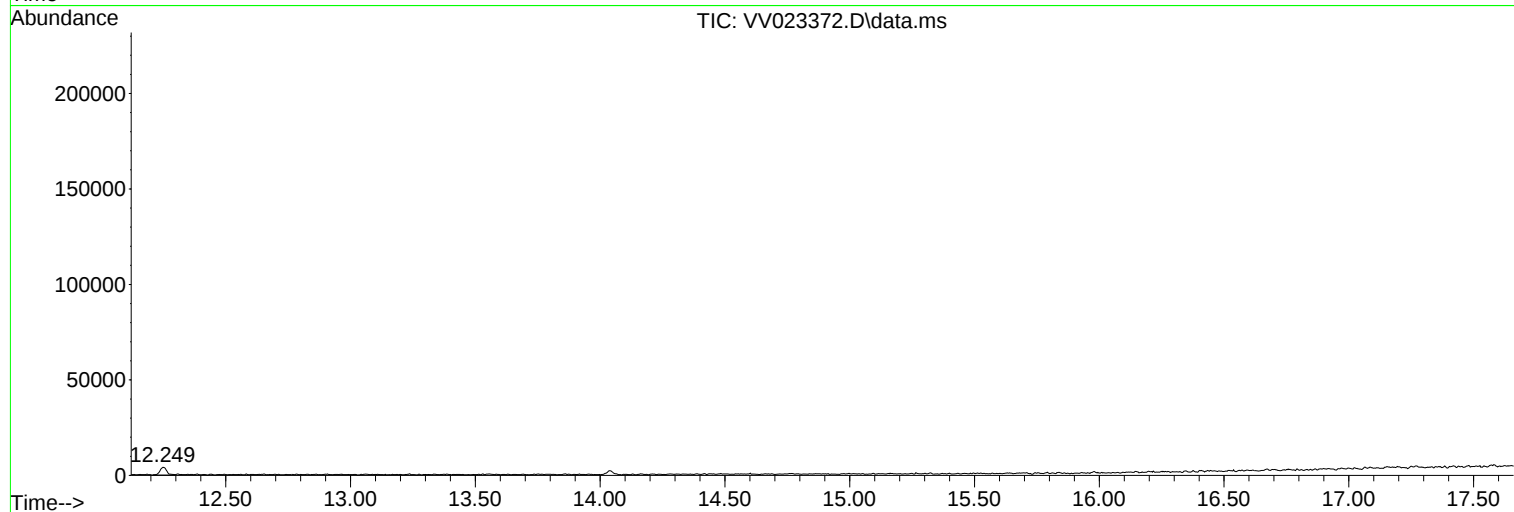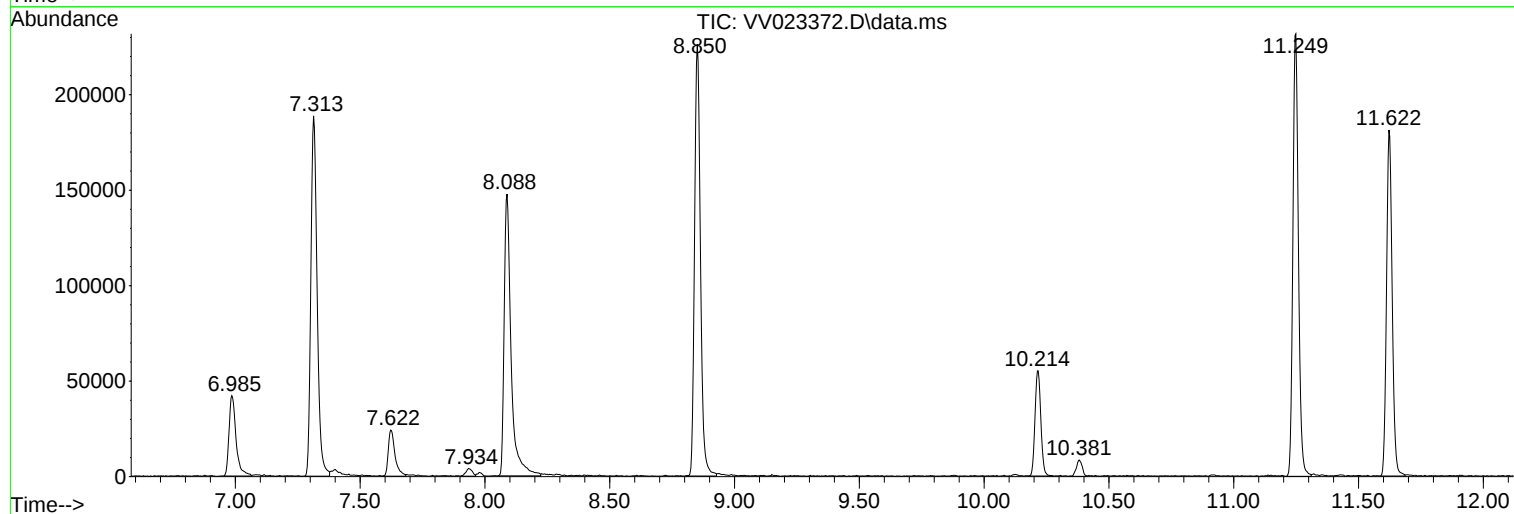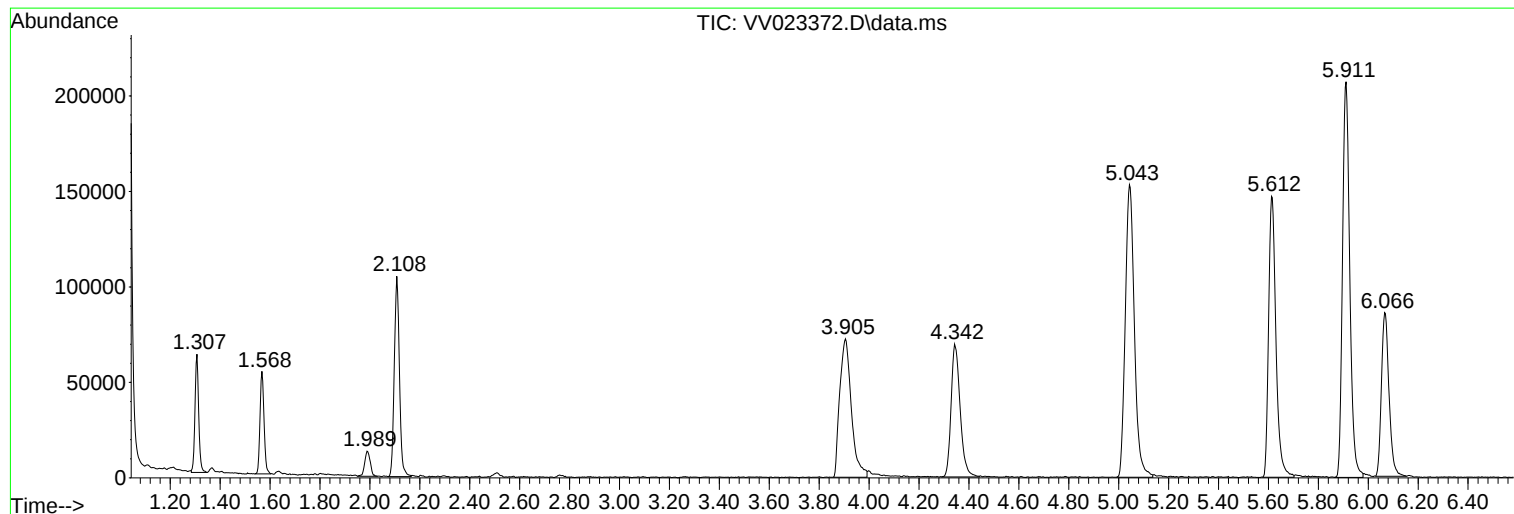

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023372.D
Acq On : 11 Nov 2021 08:47
Operator : SY/MD
Sample : M4558-11DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB873DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023372.D
Acq On : 11 Nov 2021 08:47
Operator : SY/MD
Sample : M4558-11DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 58 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB873DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc