

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
 Data File : VV023374.D
 Acq On : 11 Nov 2021 09:33
 Operator : SY/MD
 Sample : M4558-16DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB878DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023374.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	44	50	61	rVB	45265	41713	10.83%	1.128%
2	1.307	75	83	92	rBV	53761	56279	14.61%	1.521%
3	1.365	95	101	110	rVB2	9666	11202	2.91%	0.303%
4	1.568	157	164	175	rVB	46739	52260	13.57%	1.413%
5	1.992	287	296	307	rBV2	12719	19108	4.96%	0.517%
6	2.108	322	332	349	rBV	92180	134546	34.94%	3.637%
7	3.912	878	893	928	rBV3	112151	315015	81.80%	8.516%
8	4.352	1013	1030	1052	rBV	61483	159964	41.54%	4.325%
9	5.050	1231	1247	1274	rBV2	145817	367820	95.51%	9.944%
10	5.619	1413	1424	1447	rBV	139073	281742	73.16%	7.617%
11	5.915	1503	1516	1544	rBV	192030	385125	100.00%	10.412%
12	6.072	1552	1565	1591	rBV	79350	166298	43.18%	4.496%
13	6.989	1840	1850	1873	rBV2	38564	73319	19.04%	1.982%
14	7.317	1936	1952	1969	rBV	173148	305578	79.35%	8.261%
15	7.625	2039	2048	2066	rBV	22539	41335	10.73%	1.117%
16	8.092	2183	2193	2226	rBV	130190	263827	68.50%	7.132%
17	8.854	2417	2430	2452	rBV	214995	349345	90.71%	9.444%
18	10.217	2843	2854	2866	rBV	54278	84759	22.01%	2.291%
19	11.249	3164	3175	3195	rBV	213377	332459	86.32%	8.988%
20	11.625	3279	3292	3305	rBV	163971	257305	66.81%	6.956%




Sum of corrected areas: 3698999

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023374.D
Acq On : 11 Nov 2021 09:33
Operator : SY/MD
Sample : M4558-16DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB878DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

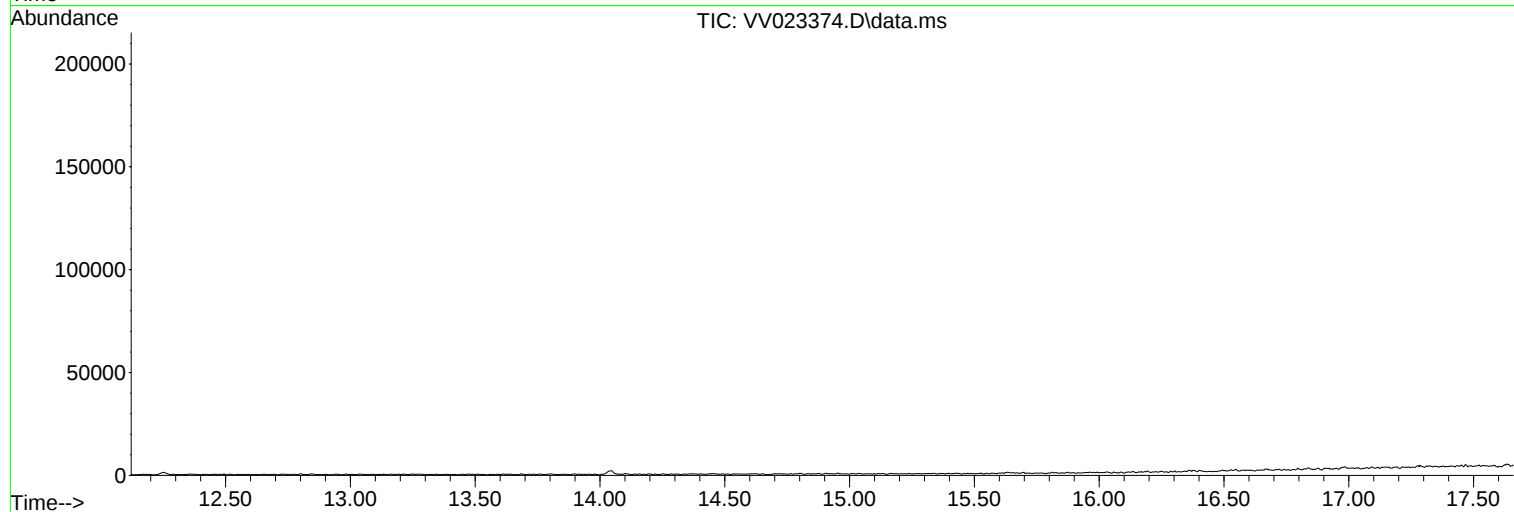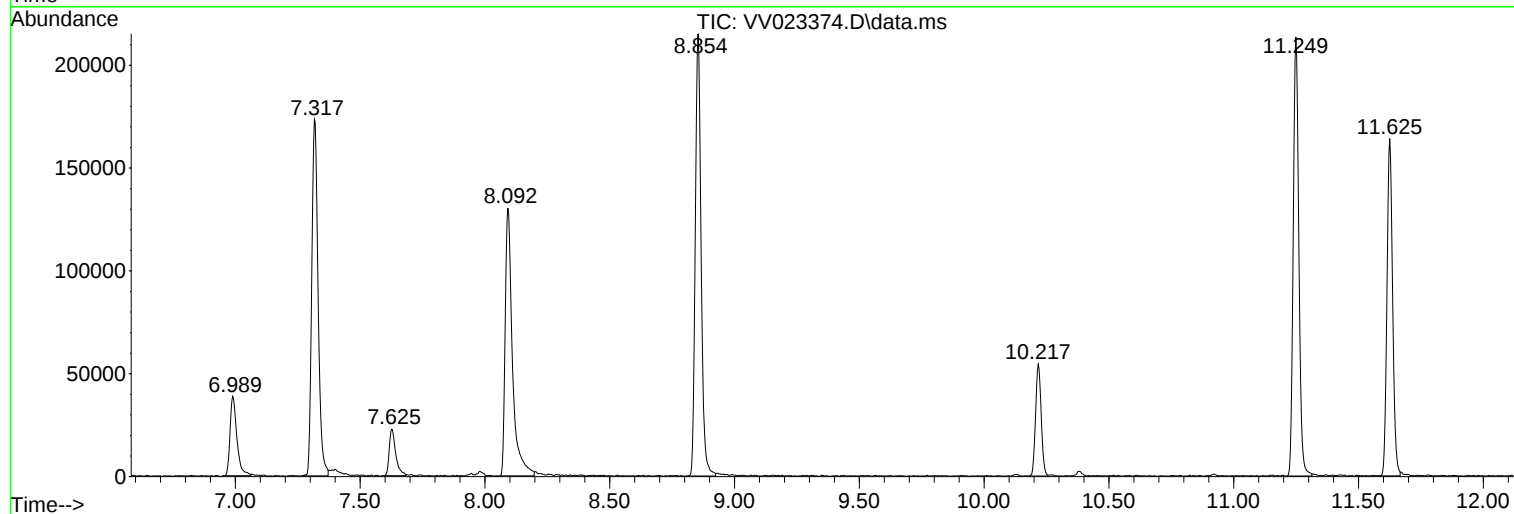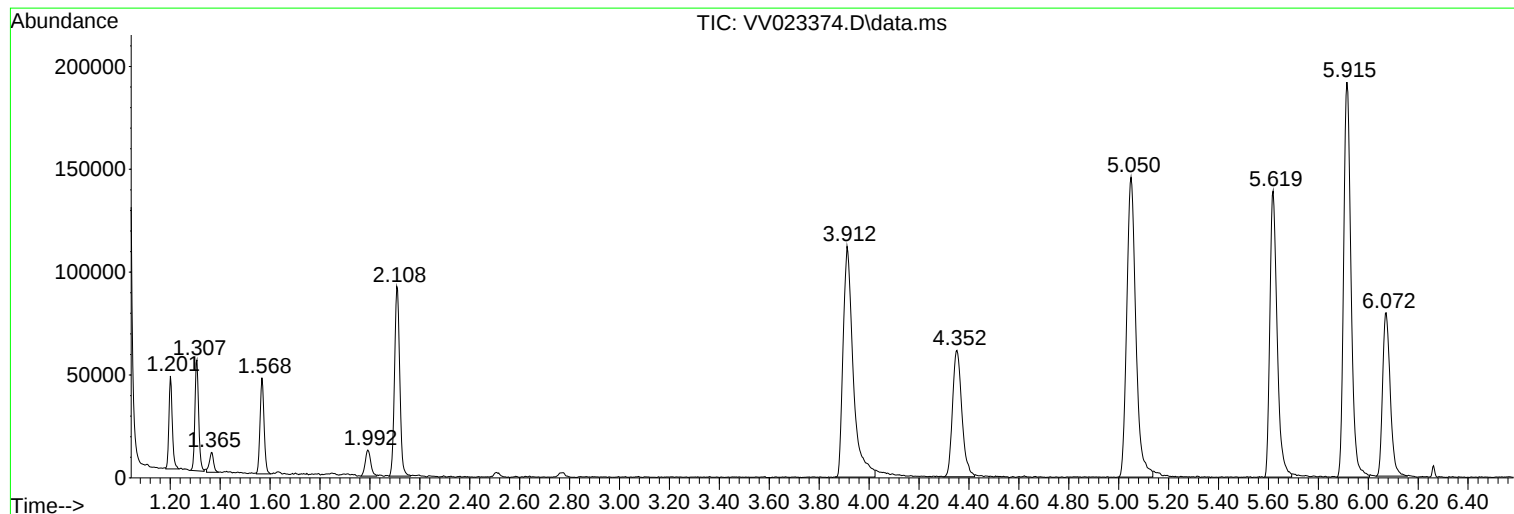

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023374.D
Acq On : 11 Nov 2021 09:33
Operator : SY/MD
Sample : M4558-16DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB878DL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.201	0.74 ug/L	41713	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Trifluoroguanidine	113	CH2F3N3	037950-72-4	9
2			Ethyne, chloro-	60	C2HC1	000593-63-5	7
3			Thiirane	60	C2H4S	000420-12-2	5
4			Methyl nitrite	61	CH3NO2	000624-91-9	5
5			o-Ethylhydroxylamine	61	C2H7NO	000624-86-2	4

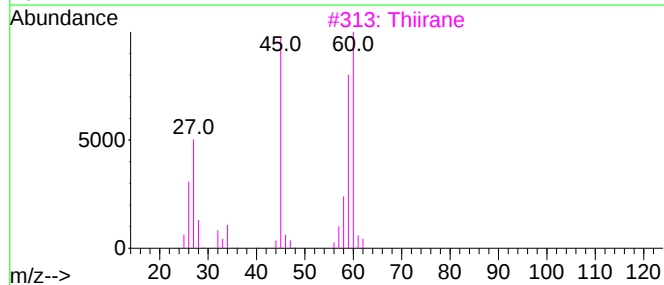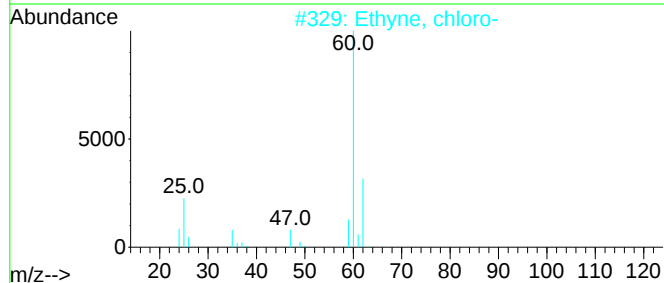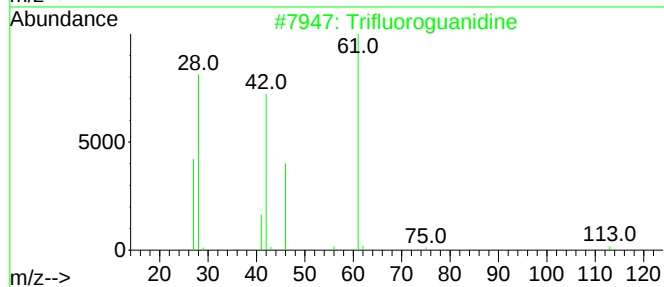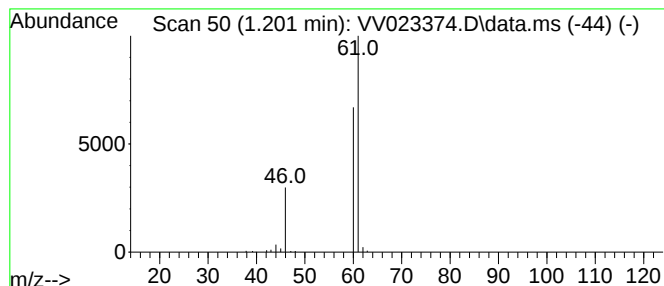

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023374.D
Acq On : 11 Nov 2021 09:33
Operator : SY/MD
Sample : M4558-16DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB878DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.201	0.7	ug/L	41713	1	5.619	281742	5.0