

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
 Data File : VV023381.D
 Acq On : 11 Nov 2021 12:37
 Operator : SY/MD
 Sample : M4558-19DL 100X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB881DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023381.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	95	rVB	53726	55702	14.09%	1.619%
2	1.568	156	164	174	rBV	45544	50408	12.75%	1.465%
3	1.992	283	296	307	rBV3	9980	15790	3.99%	0.459%
4	2.108	322	332	345	rBV	90299	131802	33.33%	3.832%
5	2.510	447	457	471	rBV2	11356	20116	5.09%	0.585%
6	3.911	881	893	929	rBV4	43153	142301	35.98%	4.137%
7	4.355	1014	1031	1059	rBV2	60585	163234	41.28%	4.745%
8	5.053	1231	1248	1268	rBV2	146794	361964	91.53%	10.523%
9	5.622	1414	1425	1450	rBV	131857	268728	67.95%	7.812%
10	5.918	1503	1517	1537	rBV	202504	395458	100.00%	11.496%
11	6.075	1551	1566	1582	rBV	82299	168947	42.72%	4.911%
12	6.992	1840	1851	1871	rBV	39623	75024	18.97%	2.181%
13	7.320	1941	1953	1971	rBV	177135	306898	77.61%	8.922%
14	7.628	2037	2049	2068	rBV3	22691	43240	10.93%	1.257%
15	7.985	2151	2160	2169	rVB6	4621	7346	1.86%	0.214%
16	8.095	2183	2194	2226	rBV	120791	249682	63.14%	7.258%
17	8.853	2420	2430	2454	rBV	202156	333859	84.42%	9.706%
18	10.217	2843	2854	2871	rBV2	52389	83633	21.15%	2.431%
19	11.249	3164	3175	3194	rBV	199707	307222	77.69%	8.931%
20	11.625	3277	3292	3315	rBV	162220	258524	65.37%	7.515%




Sum of corrected areas: 3439878

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023381.D
Acq On : 11 Nov 2021 12:37
Operator : SY/MD
Sample : M4558-19DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 68 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB881DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

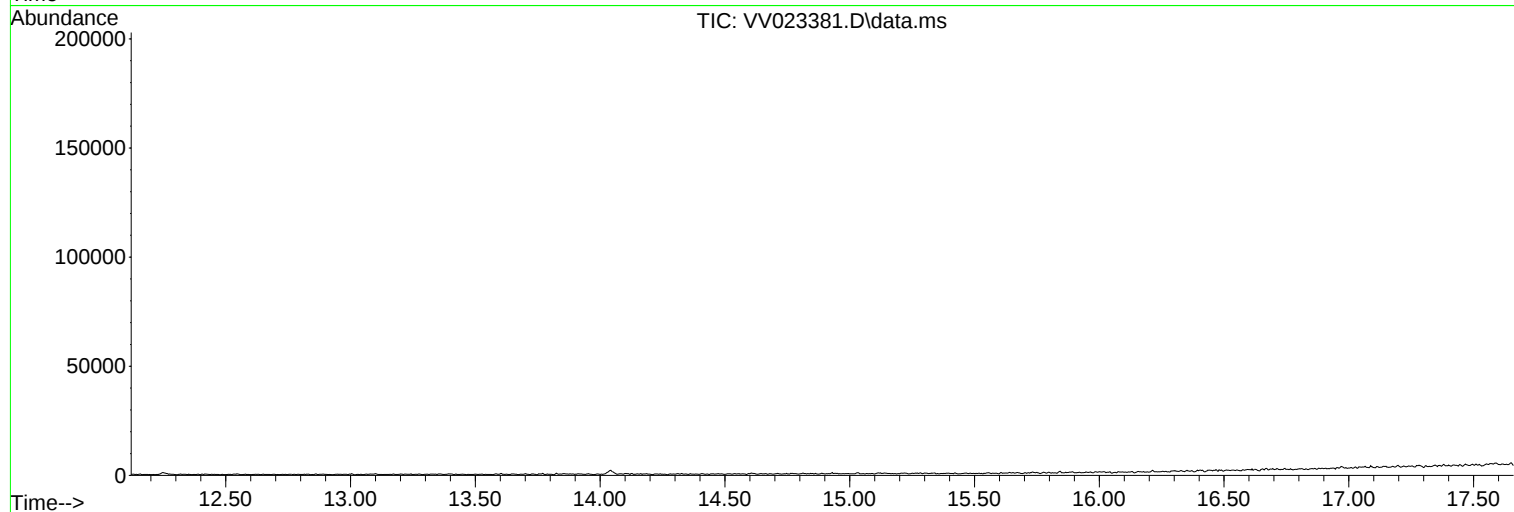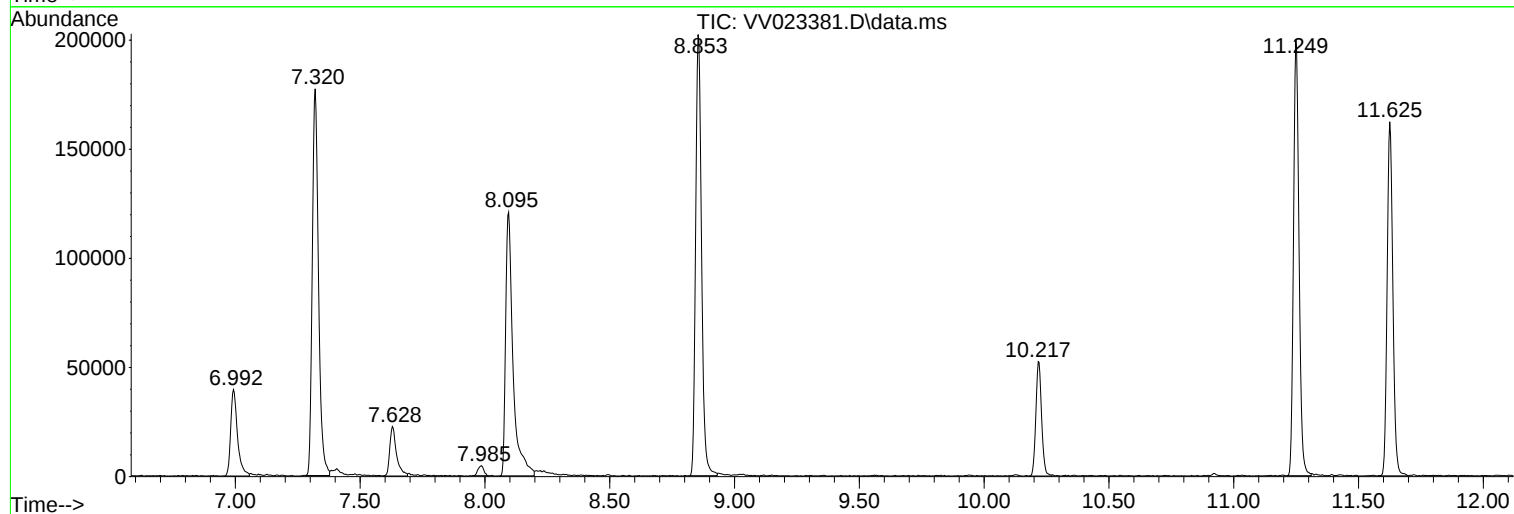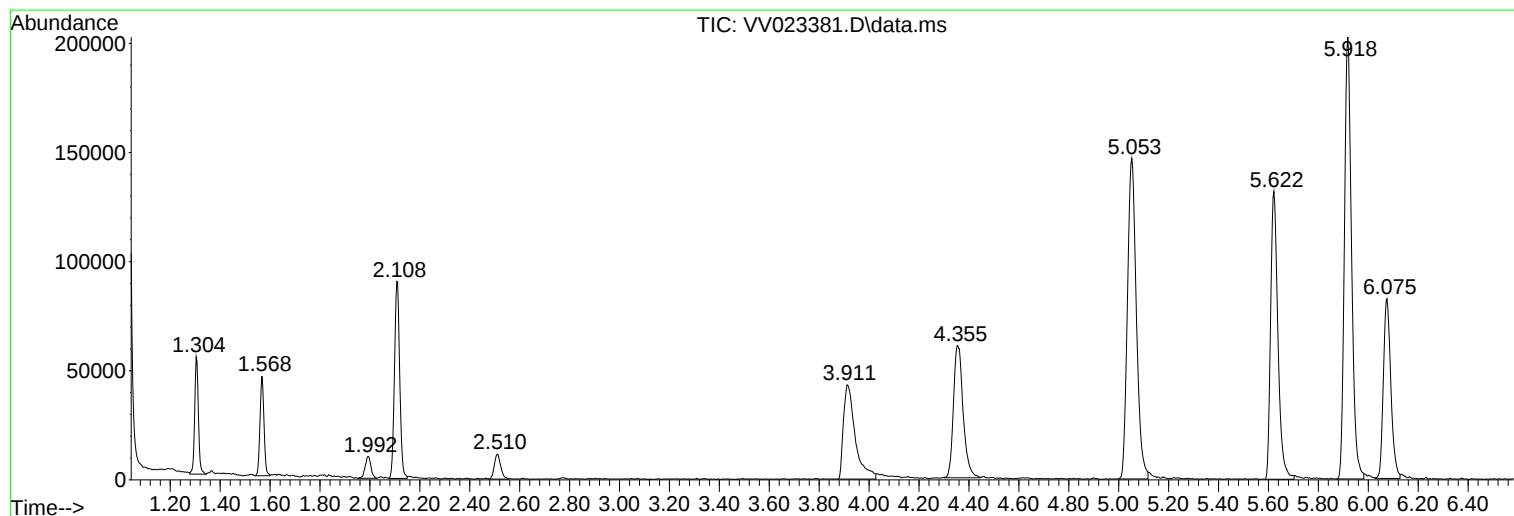

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023381.D
Acq On : 11 Nov 2021 12:37
Operator : SY/MD
Sample : M4558-19DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 68 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB881DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023381.D
Acq On : 11 Nov 2021 12:37
Operator : SY/MD
Sample : M4558-19DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 68 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB881DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc