

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
 Data File : VV023384.D
 Acq On : 11 Nov 2021 13:45
 Operator : SY/MD
 Sample : M4558-20DL 200X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB882DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023384.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	96	rVB	50087	52209	14.73%	1.597%
2	1.362	96	100	107	rBV7	3691	3701	1.04%	0.113%
3	1.564	156	163	172	rBV	44065	49605	13.99%	1.518%
4	1.989	286	295	305	rVB5	7177	11171	3.15%	0.342%
5	2.105	321	331	343	rBV	87224	124838	35.22%	3.820%
6	2.507	443	456	468	rBV4	6415	11600	3.27%	0.355%
7	3.915	882	894	929	rBV3	50339	156824	44.24%	4.798%
8	4.352	1014	1030	1052	rBV	61182	157989	44.57%	4.834%
9	5.050	1230	1247	1274	rBV2	142763	354478	100.00%	10.846%
10	5.619	1410	1424	1445	rBV2	132129	268612	75.78%	8.219%
11	5.918	1504	1517	1539	rBV	135885	277466	78.27%	8.490%
12	6.072	1553	1565	1590	rBV	80014	164303	46.35%	5.027%
13	6.992	1840	1851	1871	rBV2	37780	71717	20.23%	2.194%
14	7.320	1940	1953	1971	rBV	163633	290234	81.88%	8.880%
15	7.628	2039	2049	2070	rBV2	21732	40360	11.39%	1.235%
16	7.982	2150	2159	2172	rVB3	8777	15640	4.41%	0.479%
17	8.091	2183	2193	2231	rBV	122159	251735	71.02%	7.702%
18	8.854	2415	2430	2446	rBV	205247	331991	93.66%	10.158%
19	10.217	2844	2854	2868	rBV	53112	83473	23.55%	2.554%
20	11.249	3163	3175	3200	rBV	192720	302687	85.39%	9.261%
21	11.625	3281	3292	3312	rBV	150461	243707	68.75%	7.457%
22	14.040	4030	4043	4053	rBV3	2232	3955	1.12%	0.121%




Sum of corrected areas: 3268295

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023384.D
Acq On : 11 Nov 2021 13:45
Operator : SY/MD
Sample : M4558-20DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 71 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB882DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

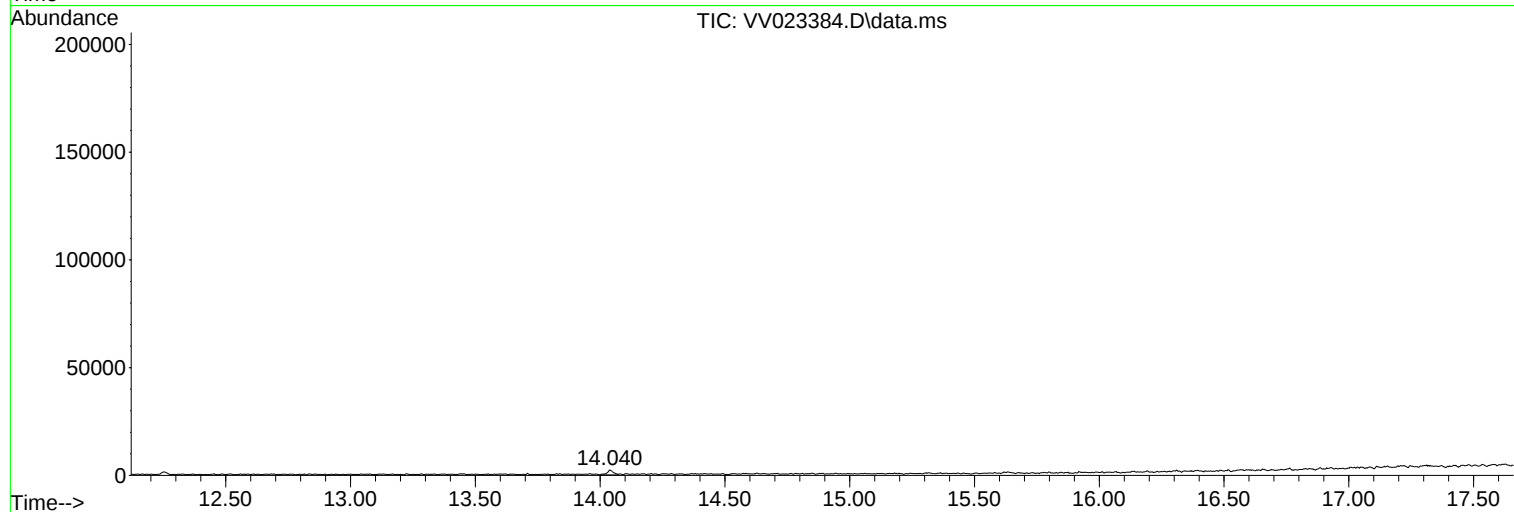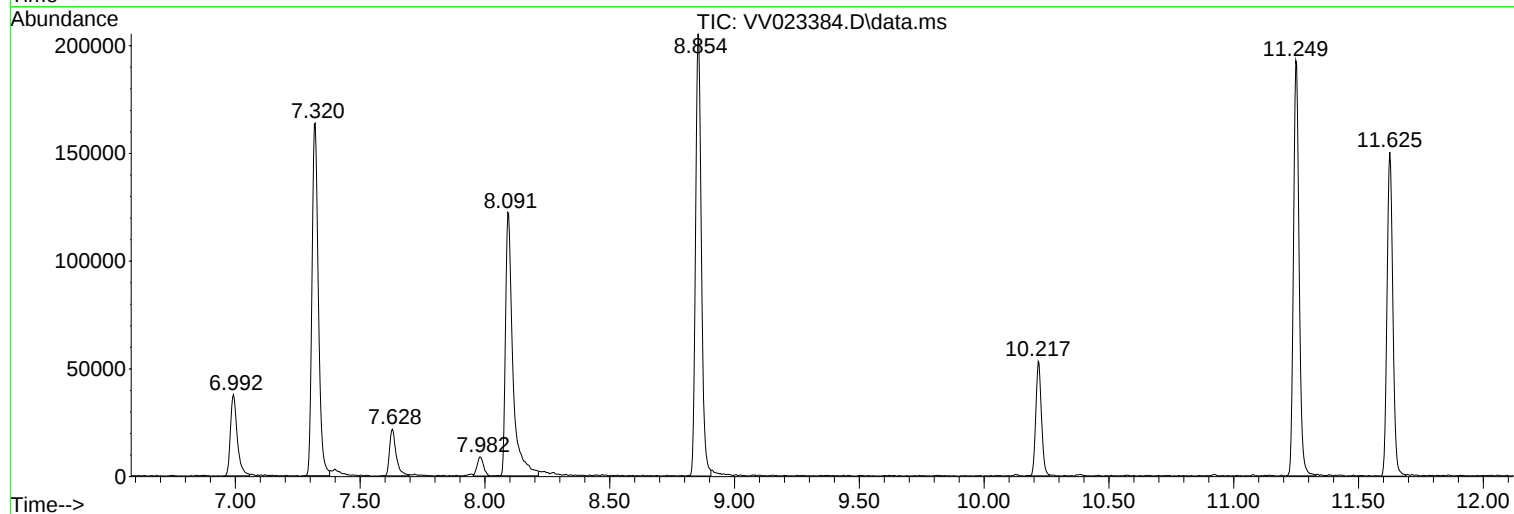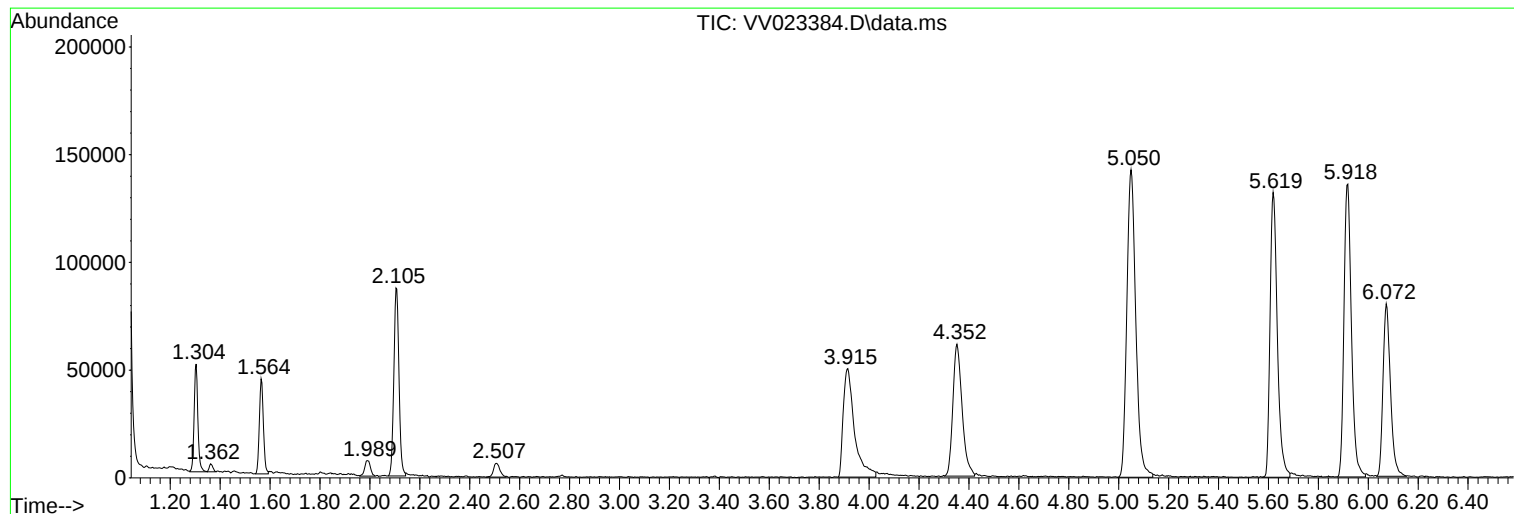

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023384.D
Acq On : 11 Nov 2021 13:45
Operator : SY/MD
Sample : M4558-20DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 71 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB882DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023384.D
Acq On : 11 Nov 2021 13:45
Operator : SY/MD
Sample : M4558-20DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 71 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB882DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
