

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
 Data File : VV023385.D
 Acq On : 11 Nov 2021 14:08
 Operator : SY/MD
 Sample : M4580-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB8G1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023385.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	97	rVB	53534	55917	16.13%	1.949%
2	1.564	156	163	172	rBV	41912	47042	13.57%	1.640%
3	2.105	321	331	343	rBV	89728	124272	35.86%	4.332%
4	3.896	878	888	919	rBV	26585	92281	26.63%	3.217%
5	4.349	1013	1029	1056	rBV	58136	152854	44.10%	5.328%
6	5.047	1231	1246	1279	rBV2	137256	346570	100.00%	12.081%
7	5.619	1412	1424	1445	rBV	121414	250262	72.21%	8.724%
8	5.915	1506	1516	1532	rVB10	3264	7264	2.10%	0.253%
9	6.069	1552	1564	1583	rBV	77554	162990	47.03%	5.682%
10	6.989	1840	1850	1870	rBV	36853	70420	20.32%	2.455%
11	7.317	1940	1952	1971	rBV	162953	287836	83.05%	10.034%
12	7.397	1973	1977	1988	rVB7	3201	5825	1.68%	0.203%
13	7.629	2037	2049	2066	rBV2	20969	39295	11.34%	1.370%
14	7.979	2148	2158	2172	rVB	28380	47948	13.84%	1.671%
15	8.092	2182	2193	2229	rBV	123518	254551	73.45%	8.873%
16	8.854	2418	2430	2459	rBV	191750	311517	89.89%	10.859%
17	10.217	2844	2854	2870	rBV	51152	82612	23.84%	2.880%
18	11.249	3164	3175	3193	rBV	177959	277580	80.09%	9.676%
19	11.532	3256	3263	3276	rBV5	4642	8882	2.56%	0.310%
20	11.625	3281	3292	3308	rBV	152968	238435	68.80%	8.311%
21	14.040	4031	4043	4053	rBV4	2338	4393	1.27%	0.153%




Sum of corrected areas: 2868746

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023385.D
Acq On : 11 Nov 2021 14:08
Operator : SY/MD
Sample : M4580-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 72 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8G1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

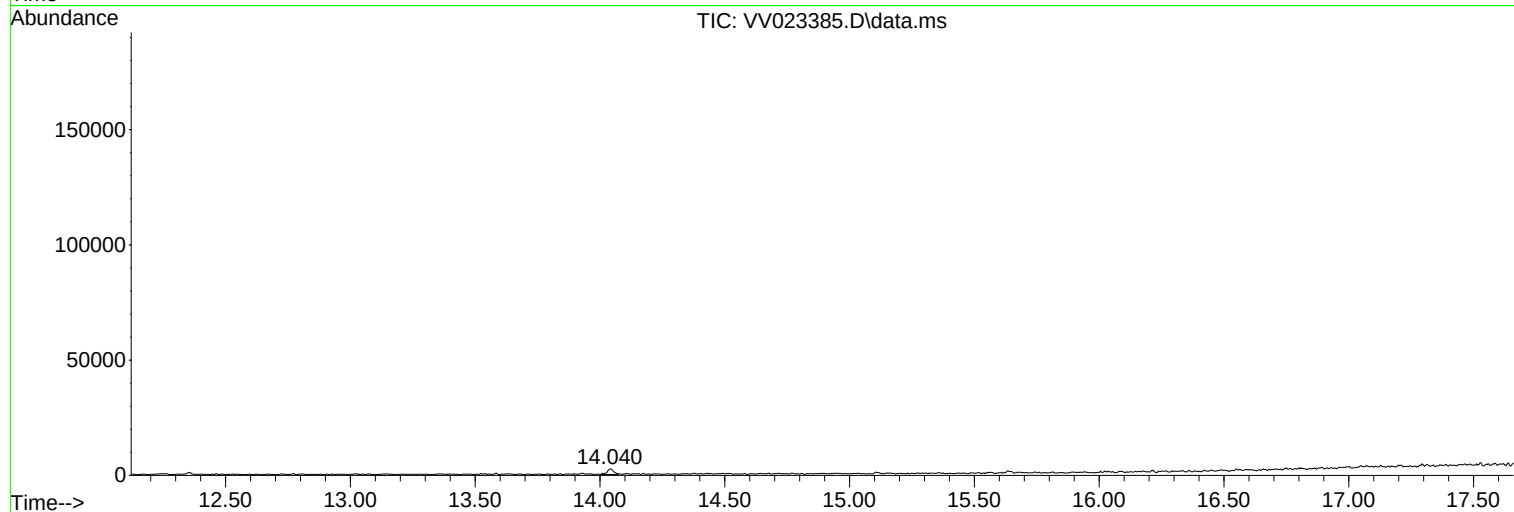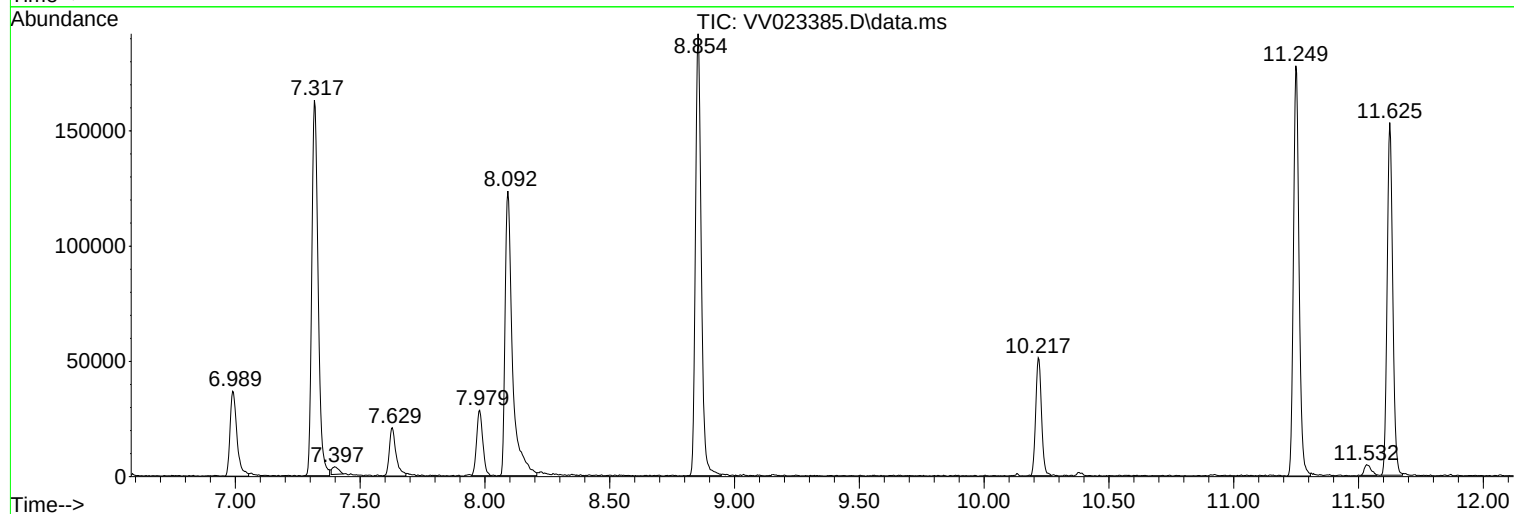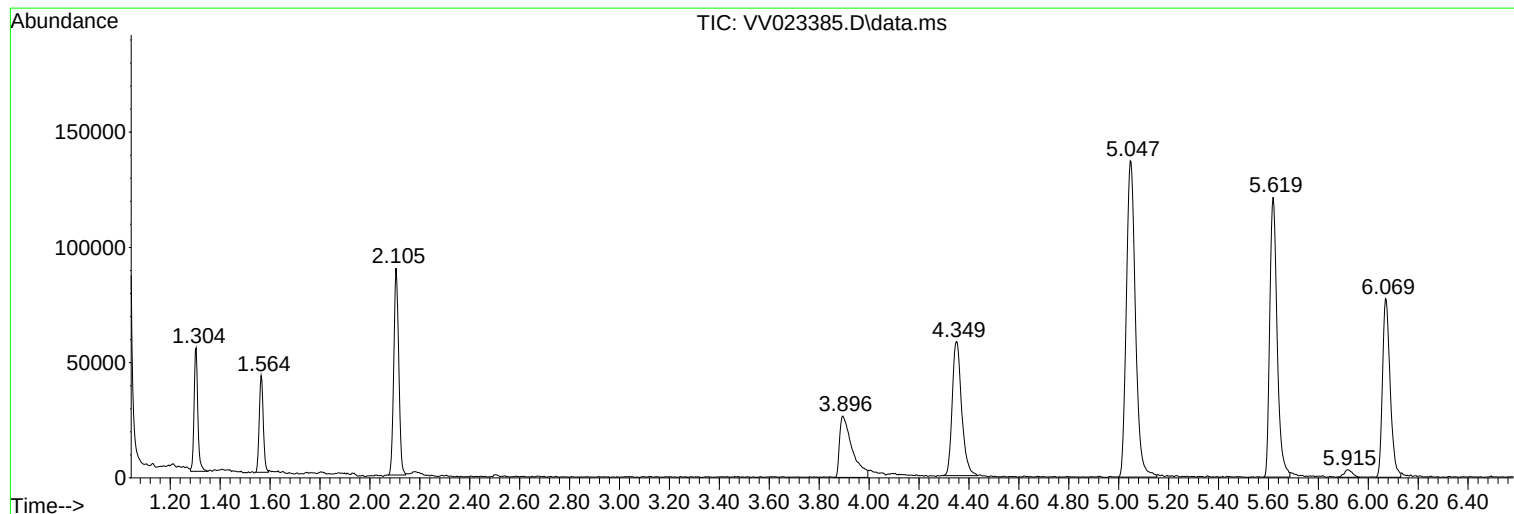

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023385.D
Acq On : 11 Nov 2021 14:08
Operator : SY/MD
Sample : M4580-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 72 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8G1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023385.D
Acq On : 11 Nov 2021 14:08
Operator : SY/MD
Sample : M4580-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 72 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8G1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
