

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
 Data File : VV023387.D
 Acq On : 11 Nov 2021 14:56
 Operator : SY/MD
 Sample : M4558-18DL 400X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB880DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023387.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rVB	54589	55870	14.09%	1.589%
2	1.568	156	164	177	rBV	42688	51665	13.03%	1.469%
3	2.105	321	331	347	rBV	89797	130626	32.94%	3.715%
4	2.507	445	456	467	rVB3	5304	9537	2.40%	0.271%
5	3.912	880	893	921	rBV5	44797	143380	36.16%	4.078%
6	4.352	1013	1030	1055	rBV3	59119	163005	41.10%	4.636%
7	5.050	1231	1247	1274	rBV2	150217	372353	93.89%	10.590%
8	5.619	1413	1424	1450	rBV	135789	278040	70.11%	7.907%
9	5.915	1503	1516	1548	rBV	201939	396567	100.00%	11.278%
10	6.072	1553	1565	1582	rBV	83891	175591	44.28%	4.994%
11	6.989	1840	1850	1866	rBV2	40338	75253	18.98%	2.140%
12	7.317	1941	1952	1971	rBV	173003	305643	77.07%	8.692%
13	7.625	2039	2048	2066	rBV	24044	44228	11.15%	1.258%
14	8.092	2182	2193	2235	rBV	144214	311525	78.56%	8.860%
15	8.854	2419	2430	2450	rBV	210601	343051	86.51%	9.756%
16	10.217	2843	2854	2870	rBV2	58786	94672	23.87%	2.692%
17	11.249	3164	3175	3199	rBV	195212	303325	76.49%	8.626%
18	11.625	3281	3292	3315	rBV	162286	257465	64.92%	7.322%
19	14.043	4032	4044	4053	rBV3	2458	4427	1.12%	0.126%




Sum of corrected areas: 3516223

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023387.D
Acq On : 11 Nov 2021 14:56
Operator : SY/MD
Sample : M4558-18DL 400X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 74 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB880DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

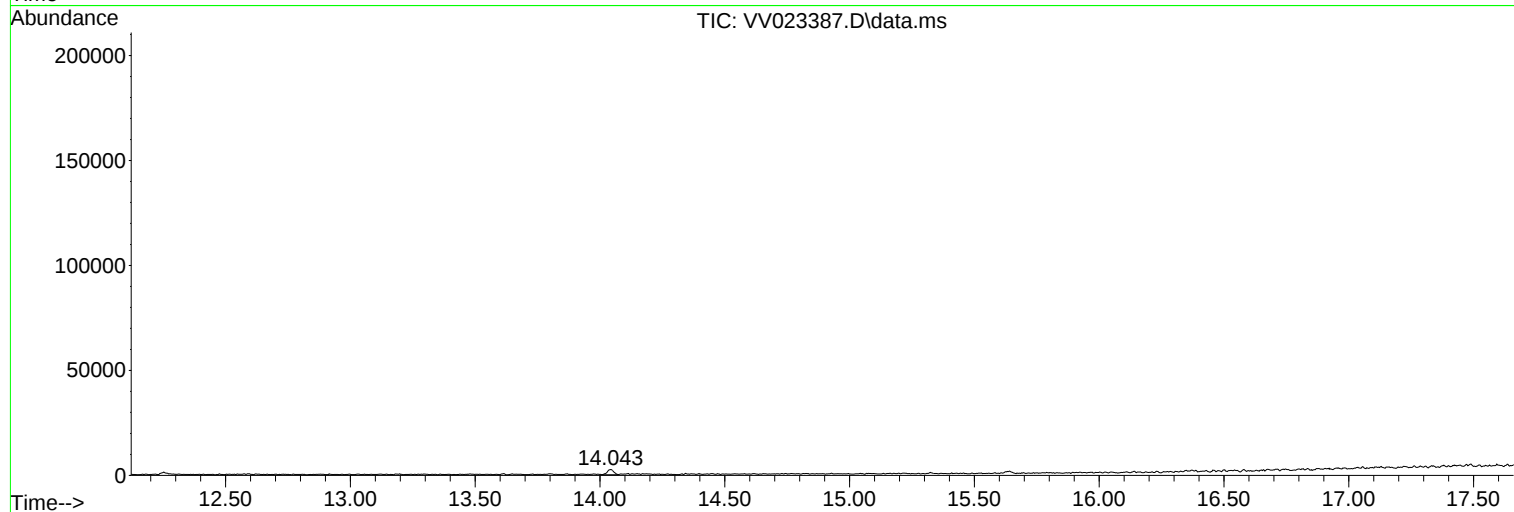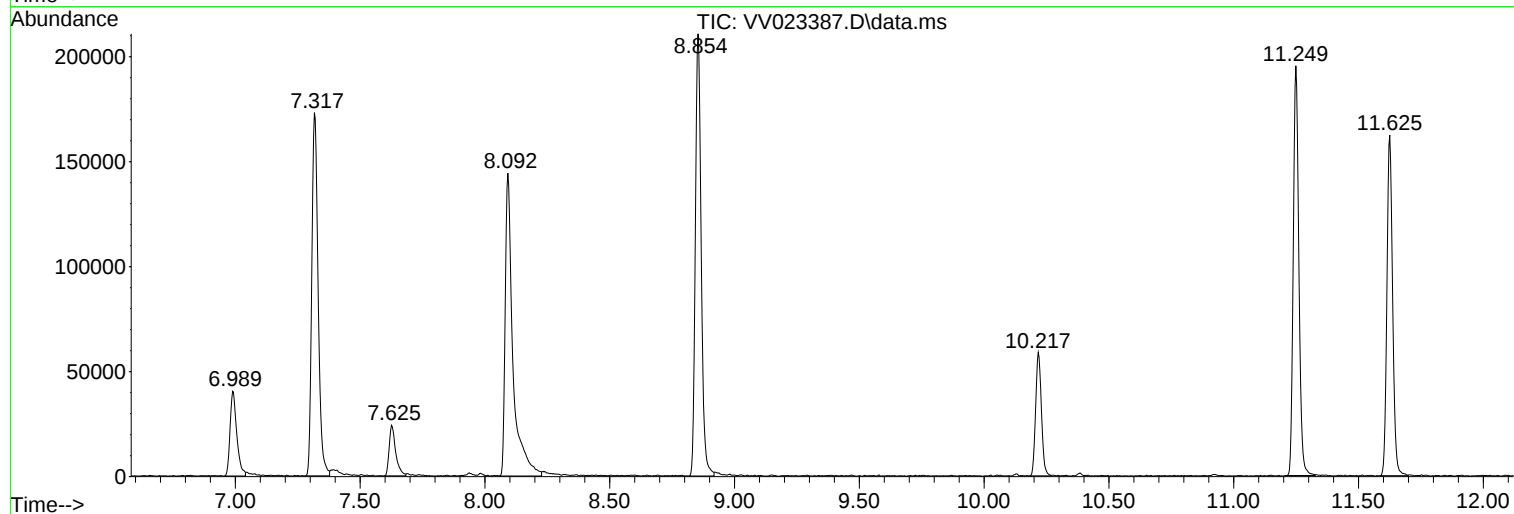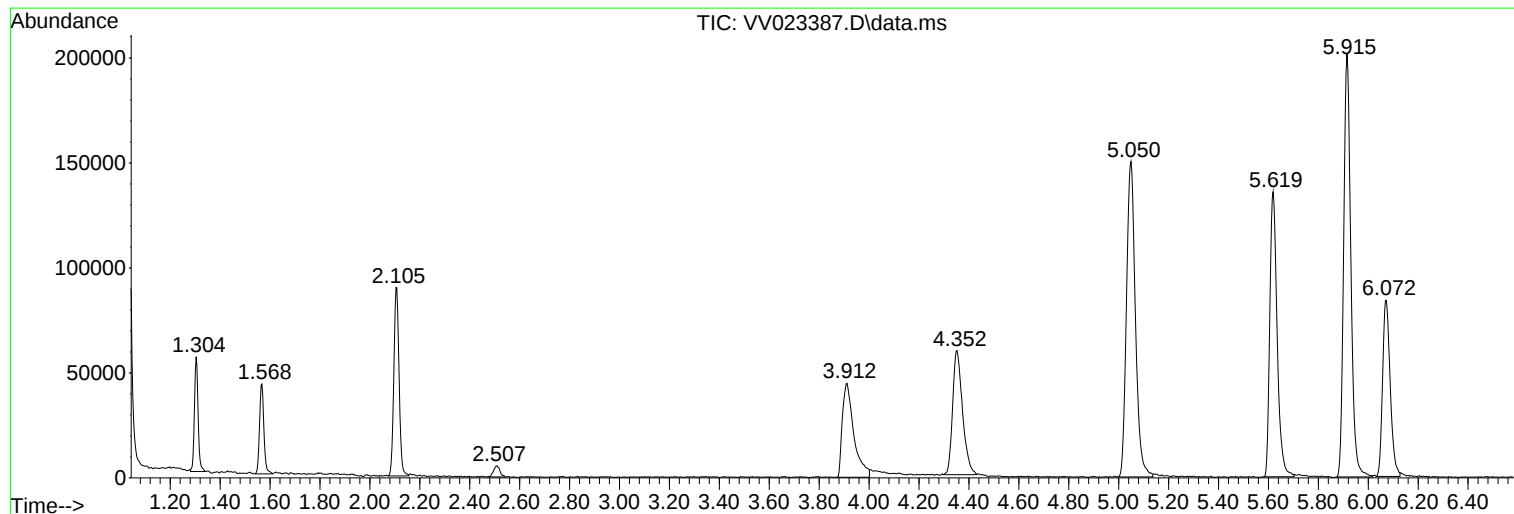

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023387.D
Acq On : 11 Nov 2021 14:56
Operator : SY/MD
Sample : M4558-18DL 400X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 74 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB880DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023387.D
Acq On : 11 Nov 2021 14:56
Operator : SY/MD
Sample : M4558-18DL 400X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 74 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB880DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc