

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
 Data File : VV023388.D
 Acq On : 11 Nov 2021 15:19
 Operator : SY/MD
 Sample : M4581-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB8J2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023388.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	74	82	99	rVB	57883	58260	15.34%	1.873%
2	1.568	156	164	178	rBV	45230	51845	13.65%	1.667%
3	2.105	321	331	343	rBV	90649	130718	34.42%	4.203%
4	3.902	881	890	927	rBV	28696	104010	27.38%	3.344%
5	4.352	1013	1030	1056	rVB	61284	166660	43.88%	5.359%
6	5.050	1230	1247	1277	rBV4	152024	379820	100.00%	12.213%
7	5.619	1410	1424	1444	rBV	130138	264400	69.61%	8.502%
8	5.918	1508	1517	1530	rVB9	3724	7822	2.06%	0.252%
9	6.072	1551	1565	1583	rBV	86670	175909	46.31%	5.656%
10	6.992	1840	1851	1878	rBV	39712	76764	20.21%	2.468%
11	7.317	1941	1952	1971	rBV	177200	309004	81.36%	9.936%
12	7.397	1971	1977	1987	rVB4	3564	6772	1.78%	0.218%
13	7.629	2039	2049	2065	rBV	24613	44386	11.69%	1.427%
14	7.979	2149	2158	2176	rVB3	14014	25254	6.65%	0.812%
15	8.092	2183	2193	2233	rBV	145052	317396	83.56%	10.206%
16	8.854	2418	2430	2449	rBV	201007	330094	86.91%	10.614%
17	10.217	2843	2854	2870	rBV2	58866	97017	25.54%	3.120%
18	10.381	2898	2905	2916	rVB5	2773	3830	1.01%	0.123%
19	11.249	3165	3175	3194	rBV	188324	294191	77.46%	9.460%
20	11.625	3279	3292	3313	rBV	165426	261110	68.75%	8.396%
21	14.037	4033	4042	4055	rBV5	2389	4734	1.25%	0.152%




Sum of corrected areas: 3109996

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023388.D
Acq On : 11 Nov 2021 15:19
Operator : SY/MD
Sample : M4581-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 75 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8J2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

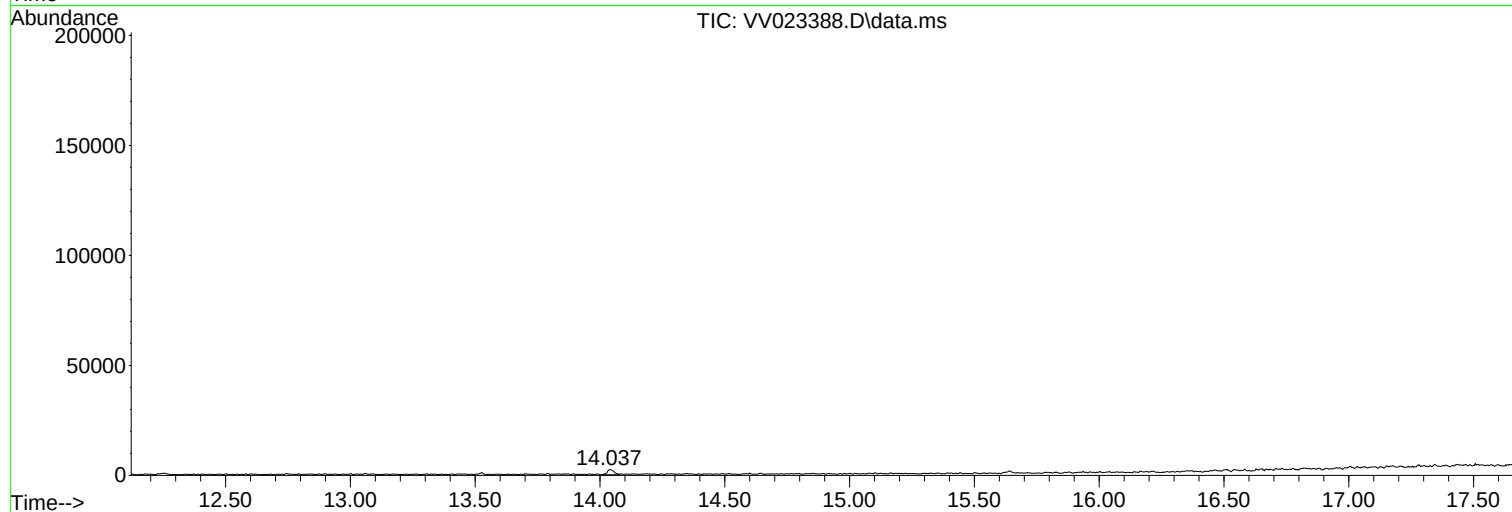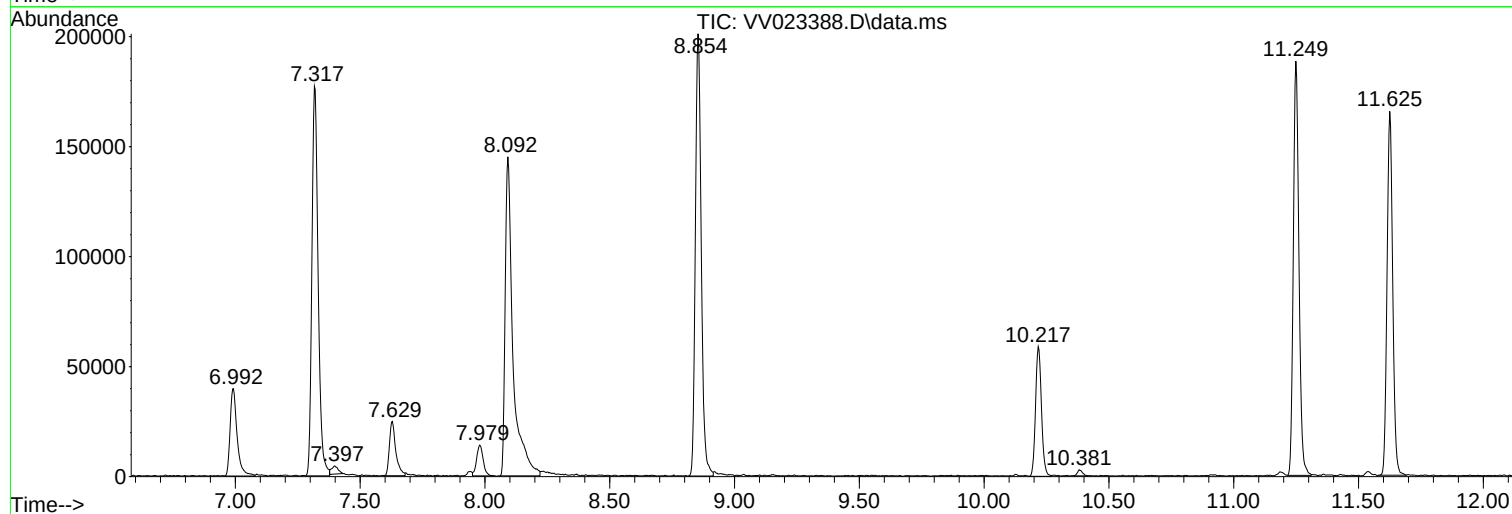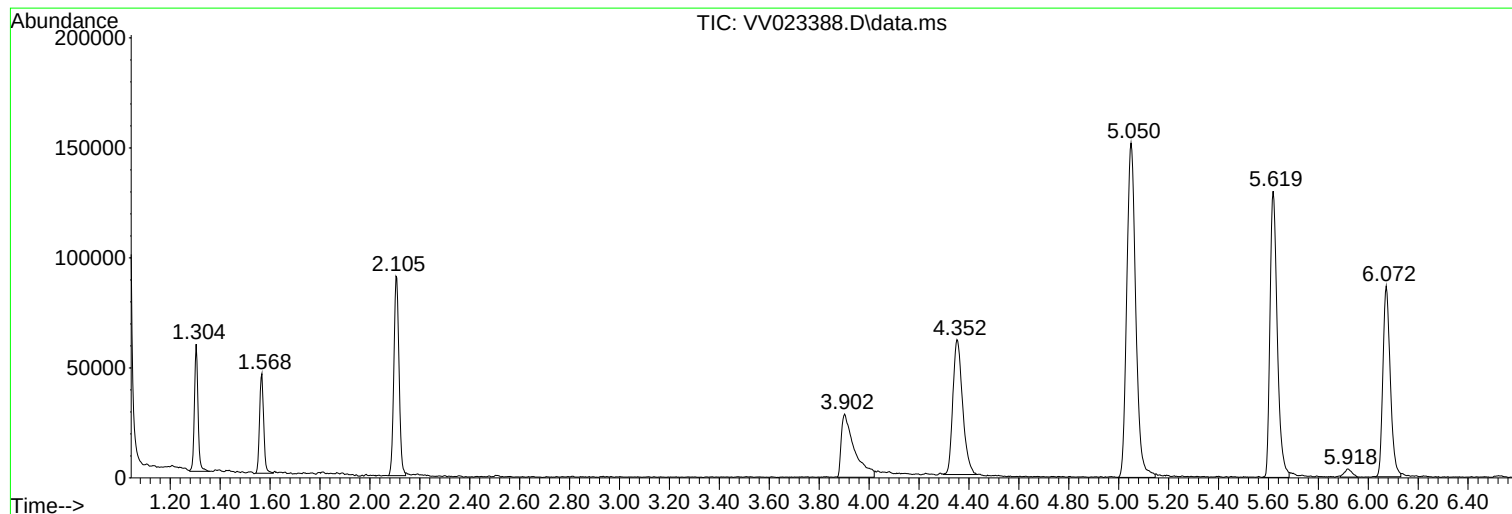

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023388.D
Acq On : 11 Nov 2021 15:19
Operator : SY/MD
Sample : M4581-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 75 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8J2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023388.D
Acq On : 11 Nov 2021 15:19
Operator : SY/MD
Sample : M4581-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 75 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8J2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
