

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
 Data File : VV023402.D
 Acq On : 11 Nov 2021 20:59
 Operator : SY/MD
 Sample : M4542-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGGF7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023402.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	74	83	96	rVB	51285	55759	15.20%	1.770%
2	1.568	155	164	172	rBV	45250	50326	13.72%	1.598%
3	2.108	321	332	345	rBV	84890	124530	33.95%	3.954%
4	2.179	345	354	367	rVV	4604	9746	2.66%	0.309%
5	3.693	808	825	838	rBV8	2528	6898	1.88%	0.219%
6	3.892	878	887	921	rBV2	36455	122895	33.50%	3.902%
7	4.349	1010	1029	1056	rBV	63060	160164	43.66%	5.086%
8	5.050	1230	1247	1272	rBV2	144857	366827	100.00%	11.648%
9	5.619	1412	1424	1447	rBV2	135043	272422	74.26%	8.650%
10	5.908	1504	1514	1529	rVB10	4126	8899	2.43%	0.283%
11	6.069	1551	1564	1584	rBV	82398	172358	46.99%	5.473%
12	6.989	1839	1850	1869	rBV	37406	72162	19.67%	2.291%
13	7.317	1938	1952	1971	rBV	170838	299470	81.64%	9.509%
14	7.397	1971	1977	1992	rVB3	4262	8483	2.31%	0.269%
15	7.625	2039	2048	2071	rBV2	22454	43716	11.92%	1.388%
16	7.941	2134	2146	2157	rBV3	3525	6396	1.74%	0.203%
17	8.092	2182	2193	2228	rBV	157189	311006	84.78%	9.875%
18	8.854	2419	2430	2446	rBV	203855	334141	91.09%	10.610%
19	10.217	2843	2854	2871	rBV	56246	88438	24.11%	2.808%
20	10.384	2897	2906	2916	rVB3	6041	9421	2.57%	0.299%
21	11.249	3164	3175	3197	rBV	194785	306523	83.56%	9.733%
22	11.532	3254	3263	3274	rBV3	14099	24337	6.63%	0.773%
23	11.625	3281	3292	3308	rBV	165532	262900	71.67%	8.348%
24	12.252	3478	3487	3495	rBV3	3441	5508	1.50%	0.175%
25	12.345	3504	3516	3529	rBV4	10542	16518	4.50%	0.524%
26	14.043	4032	4044	4054	rBV	3171	5595	1.53%	0.178%
27	15.117	4370	4378	4389	rVB5	2792	3933	1.07%	0.125%




Sum of corrected areas: 3149371

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023402.D
Acq On : 11 Nov 2021 20:59
Operator : SY/MD
Sample : M4542-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGGF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

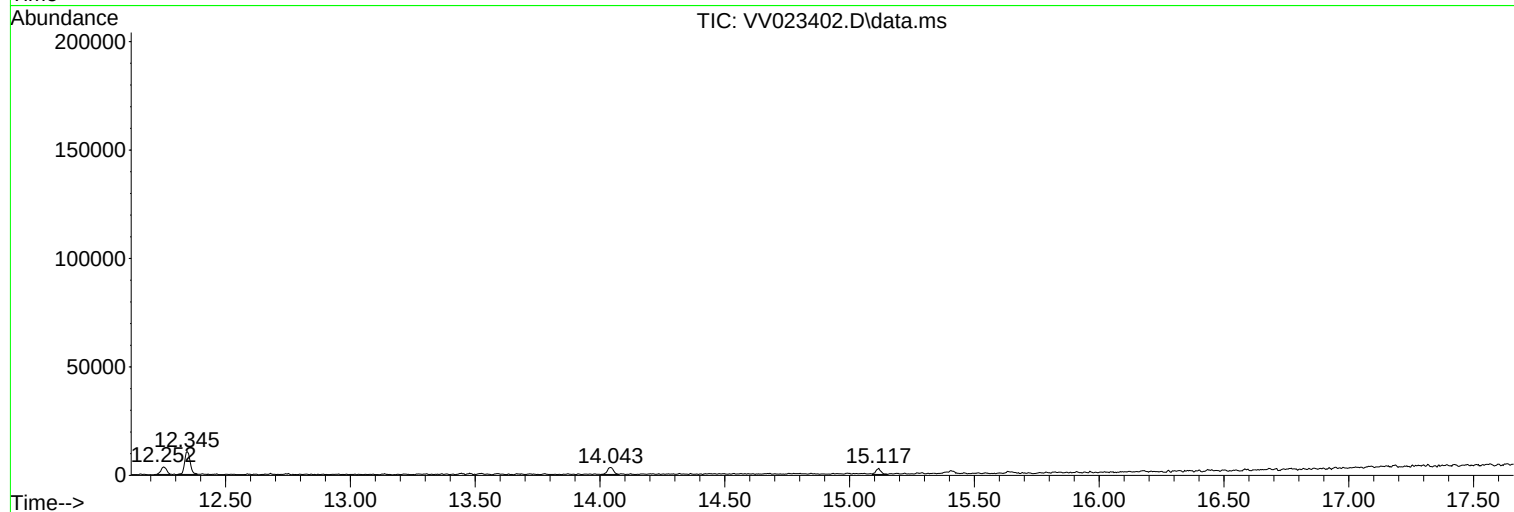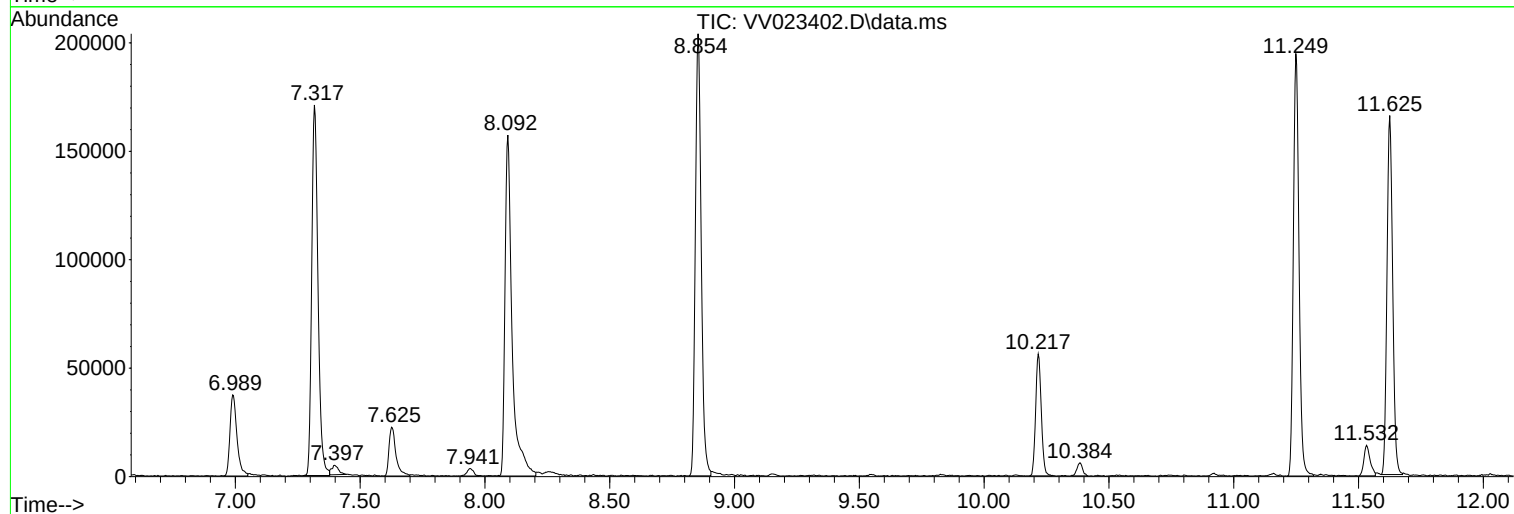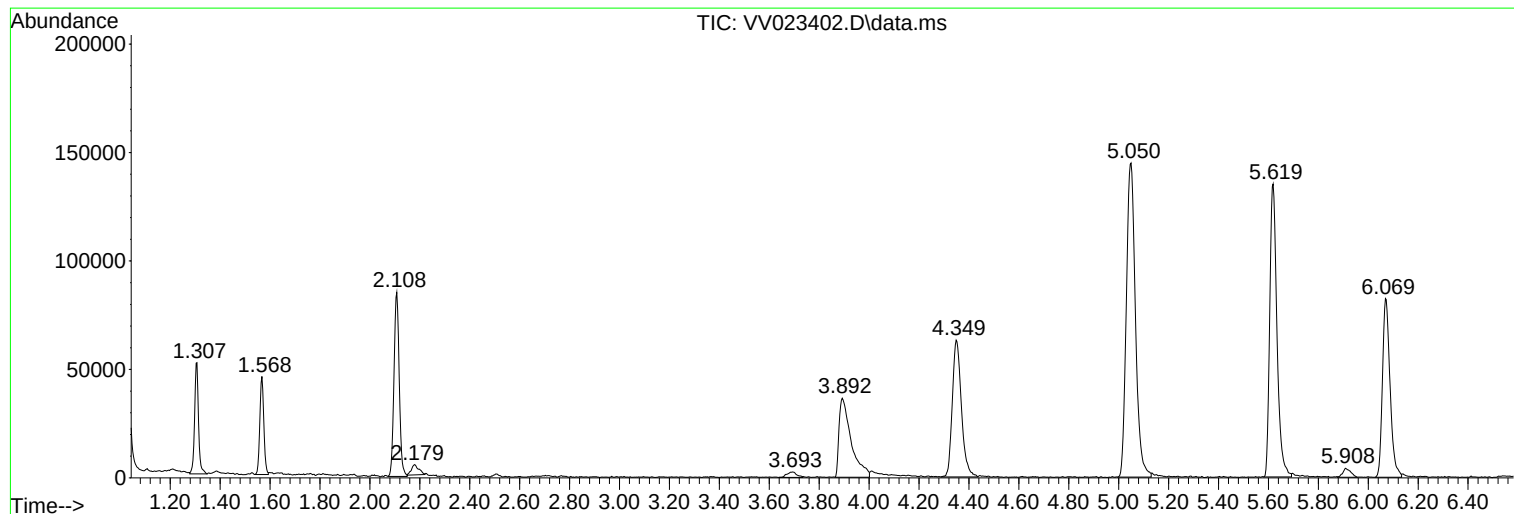

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023402.D
Acq On : 11 Nov 2021 20:59
Operator : SY/MD
Sample : M4542-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGGF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023402.D
Acq On : 11 Nov 2021 20:59
Operator : SY/MD
Sample : M4542-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGGF7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
