

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
 Data File : VV023411.D
 Acq On : 12 Nov 2021 00:35
 Operator : SY/MD
 Sample : M4580-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB8G7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023411.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.298	71	80	94	rVB	48114	47547	12.67%	1.574%
2	1.561	154	162	174	rVB	38945	46261	12.33%	1.531%
3	1.751	210	221	227	rVB4	3034	4635	1.24%	0.153%
4	2.098	320	329	342	rBV	82446	117152	31.22%	3.878%
5	3.966	892	910	933	rBV2	21521	93155	24.83%	3.083%
6	4.342	1011	1027	1046	rVB2	67221	165139	44.01%	5.466%
7	5.040	1230	1244	1269	rBV3	166975	375211	100.00%	12.419%
8	5.616	1410	1423	1445	rBV	142800	283602	75.58%	9.387%
9	5.899	1500	1511	1521	rBV8	3504	6867	1.83%	0.227%
10	6.069	1550	1564	1586	rBV3	84554	177459	47.30%	5.874%
11	6.519	1696	1704	1717	rVB6	2156	3874	1.03%	0.128%
12	6.989	1839	1850	1873	rBV	38452	71365	19.02%	2.362%
13	7.313	1938	1951	1970	rBV	166947	292590	77.98%	9.685%
14	7.625	2038	2048	2070	rBV2	22562	42334	11.28%	1.401%
15	7.976	2147	2157	2169	rVB2	17727	30963	8.25%	1.025%
16	8.104	2187	2197	2230	rBV	128358	291364	77.65%	9.644%
17	8.853	2419	2430	2446	rBV	204001	337865	90.05%	11.183%
18	10.220	2843	2855	2868	rBV	54706	88496	23.59%	2.929%
19	11.249	3159	3175	3191	rBV	185537	289288	77.10%	9.575%
20	11.538	3255	3265	3281	rBV3	7188	13922	3.71%	0.461%
21	11.625	3281	3292	3306	rVV	154806	242089	64.52%	8.013%




Sum of corrected areas: 3021178

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023411.D
Acq On : 12 Nov 2021 00:35
Operator : SY/MD
Sample : M4580-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8G7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

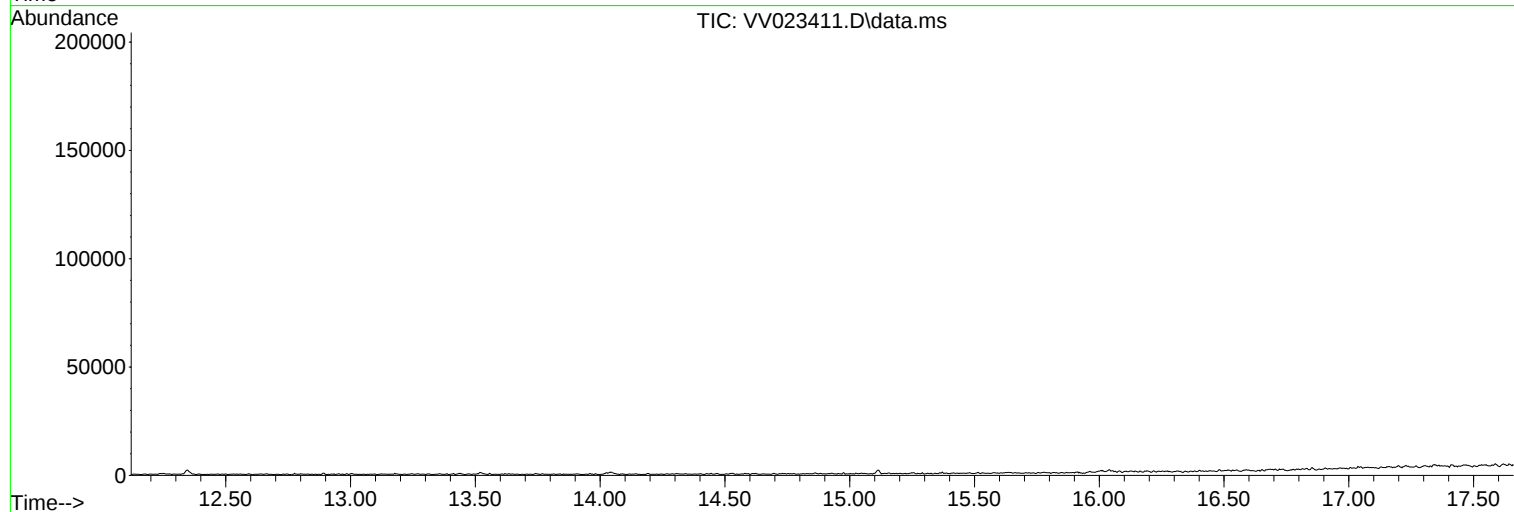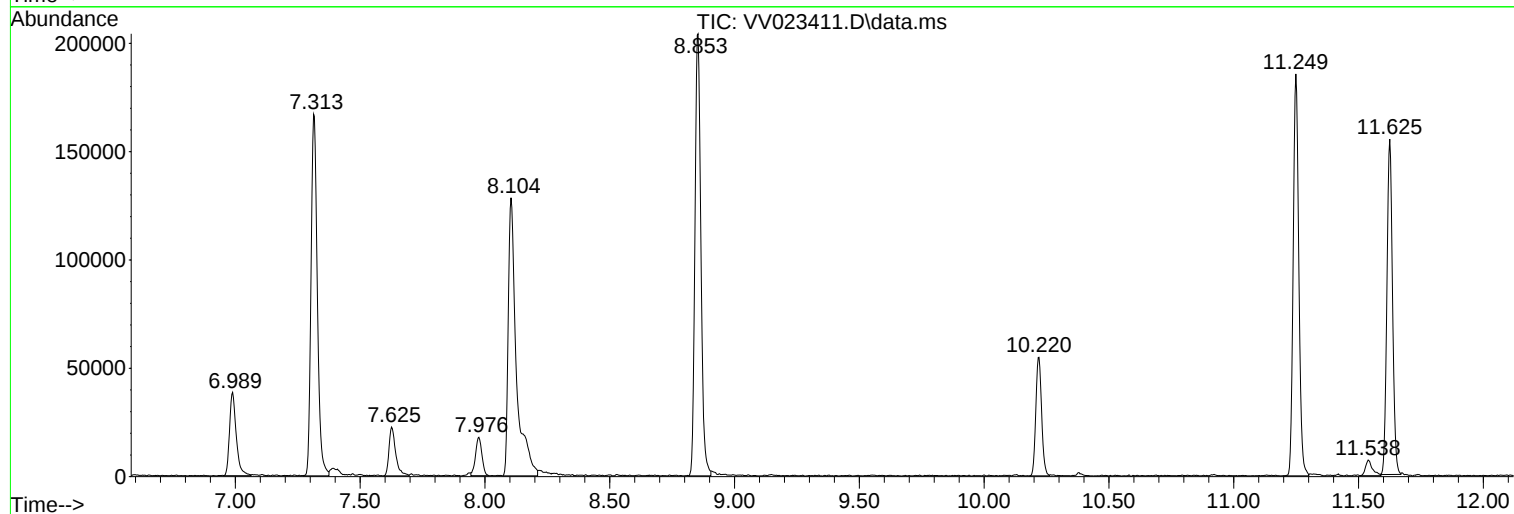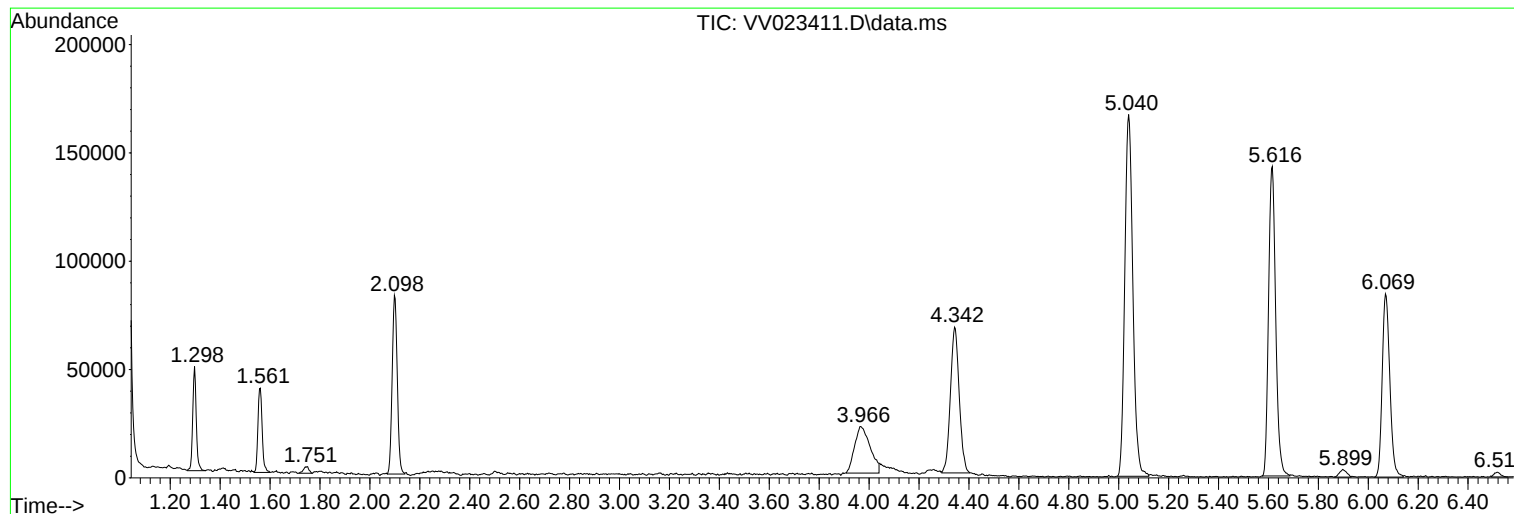

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023411.D
Acq On : 12 Nov 2021 00:35
Operator : SY/MD
Sample : M4580-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8G7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023411.D
Acq On : 12 Nov 2021 00:35
Operator : SY/MD
Sample : M4580-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8G7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc