

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
 Data File : VV023415.D
 Acq On : 12 Nov 2021 02:11
 Operator : SY/MD
 Sample : M4580-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB8H1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023415.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.298	73	80	92	rVB	42345	45169	12.25%	1.514%
2	1.558	154	161	172	rBV	41071	46321	12.56%	1.552%
3	2.098	320	329	343	rBV	80135	114665	31.09%	3.843%
4	4.002	895	921	924	rBV	17436	54434	14.76%	1.824%
5	4.343	1008	1027	1056	rVB2	62097	166986	45.28%	5.596%
6	5.037	1228	1243	1264	rBV3	166918	368814	100.00%	12.361%
7	5.613	1408	1422	1444	rBV	142552	281936	76.44%	9.449%
8	5.896	1499	1510	1521	rVB8	3991	7332	1.99%	0.246%
9	6.069	1550	1564	1584	rBV	85219	172261	46.71%	5.773%
10	6.513	1691	1702	1715	rVB2	3803	6760	1.83%	0.227%
11	6.989	1838	1850	1865	rBV	36825	67892	18.41%	2.275%
12	7.314	1940	1951	1968	rBV	157991	271500	73.61%	9.099%
13	7.397	1968	1977	1987	rVB3	3094	6060	1.64%	0.203%
14	7.625	2039	2048	2067	rBV2	22707	39863	10.81%	1.336%
15	7.973	2137	2156	2171	rVB2	56065	96915	26.28%	3.248%
16	8.108	2187	2198	2230	rBV2	126824	285523	77.42%	9.569%
17	8.850	2418	2429	2446	rBV	204379	333181	90.34%	11.166%
18	10.217	2843	2854	2870	rBV	54611	87570	23.74%	2.935%
19	11.249	3164	3175	3190	rBV	185695	283646	76.91%	9.506%
20	11.542	3256	3266	3280	rBV6	5952	11972	3.25%	0.401%
21	11.625	3280	3292	3307	rBV	147857	235002	63.72%	7.876%




Sum of corrected areas: 2983802

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023415.D
Acq On : 12 Nov 2021 02:11
Operator : SY/MD
Sample : M4580-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8H1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

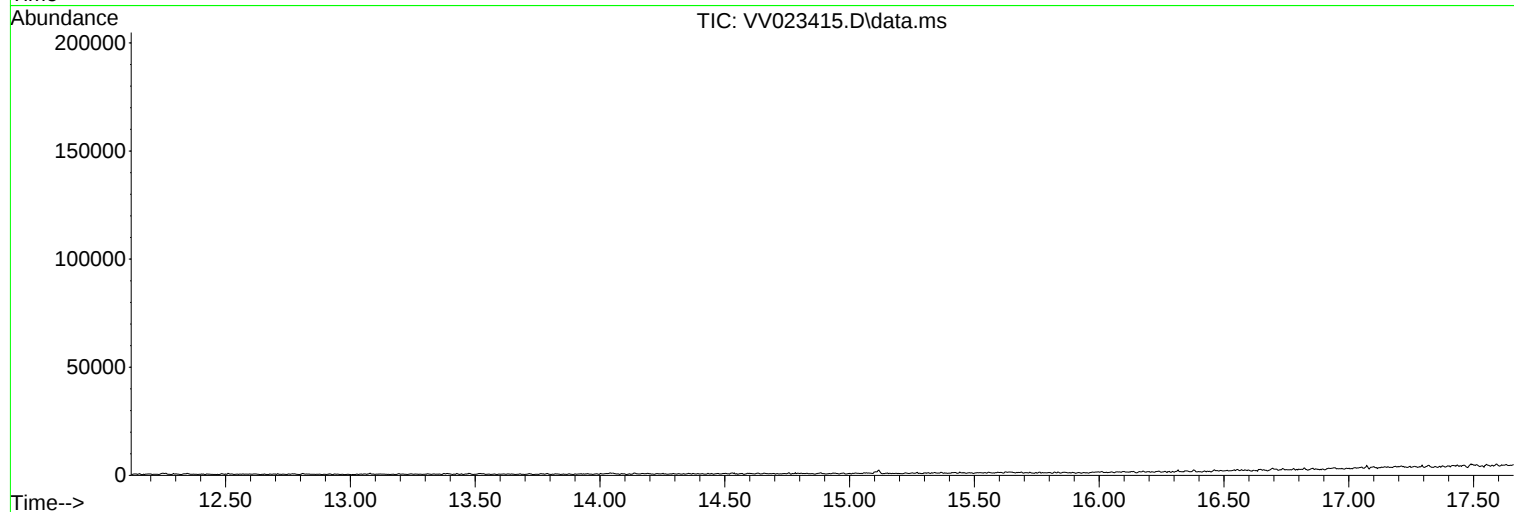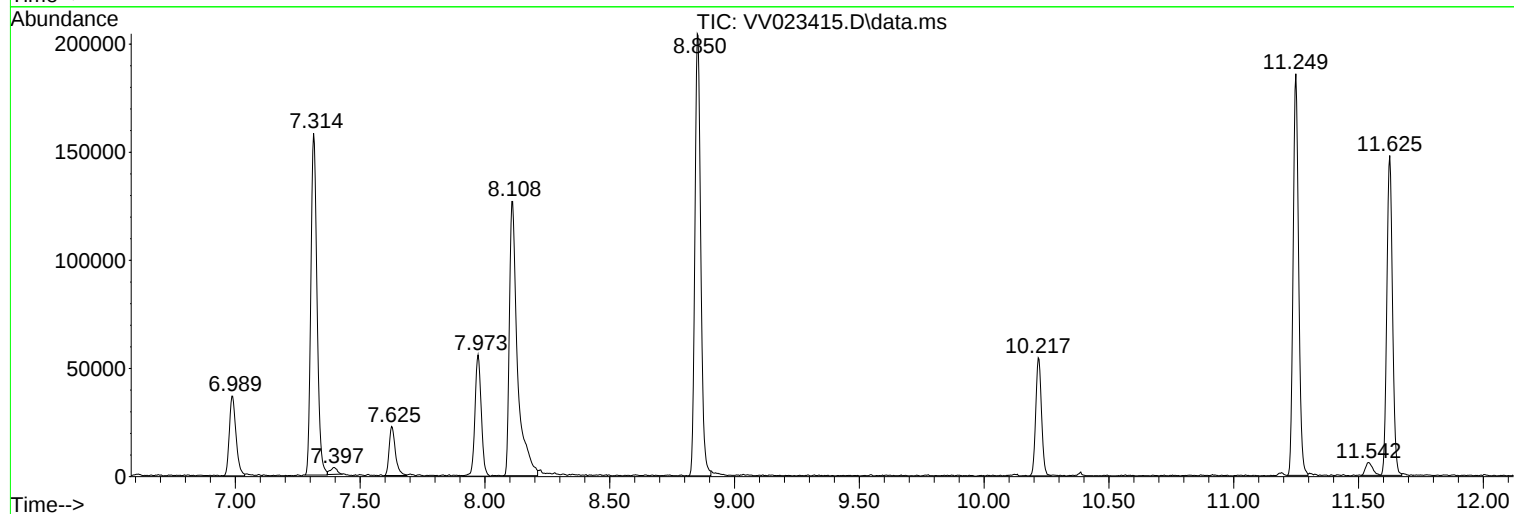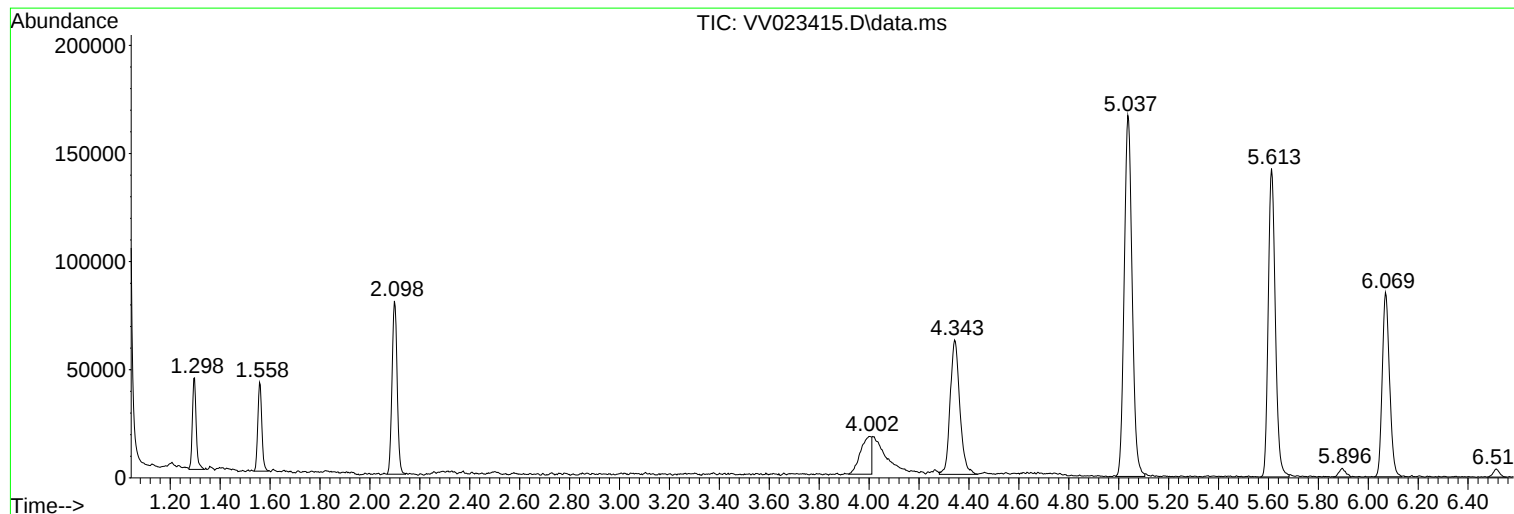

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023415.D
Acq On : 12 Nov 2021 02:11
Operator : SY/MD
Sample : M4580-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8H1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023415.D
Acq On : 12 Nov 2021 02:11
Operator : SY/MD
Sample : M4580-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8H1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc