
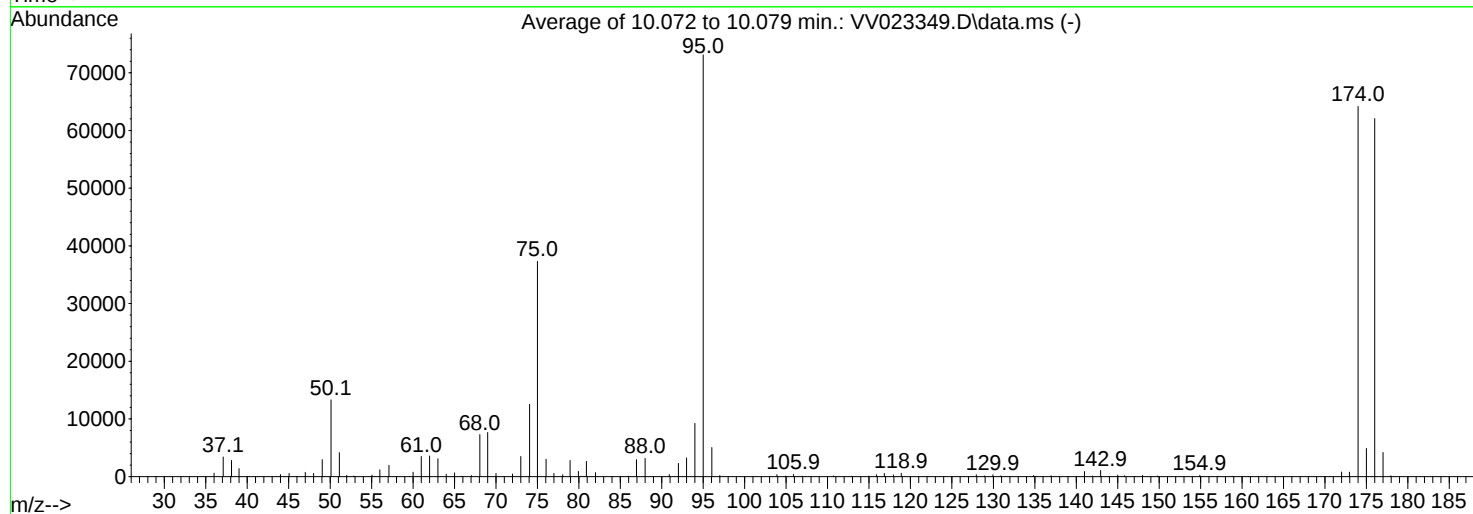


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111021\
Data File : VV023349.D
Acq On : 10 Nov 2021 22:19
Operator : SY/MD
Sample : BFB232
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB232

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Nov 17 02:49:39 2021

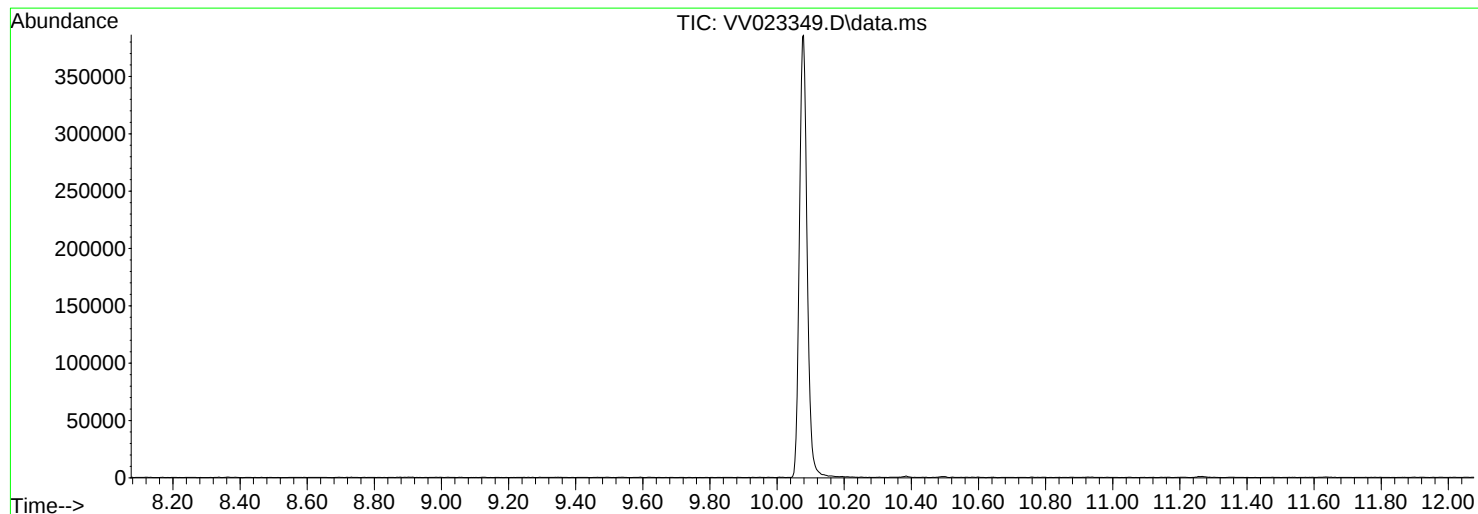

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	13324	PASS
75	95	30	80	51.0	37307	PASS
95	95	100	100	100.0	73109	PASS
96	95	5	9	6.9	5057	PASS
173	174	0.00	2	1.2	786	PASS
174	95	50	120	87.8	64181	PASS
175	174	5	9	7.6	4873	PASS
176	174	95	105	96.7	62072	PASS
177	176	5	10	6.7	4188	PASS

m/z	Abundance
40.00	211.0
44.10	268.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232

m/z	Abundance
36.00	556.0
37.10	3096.0
38.10	2607.0
39.00	1348.0
40.10	151.0
44.00	644.0
45.00	535.0
45.90	122.0
47.00	733.0
48.00	465.0
49.00	2929.0
50.10	12120.0
51.10	3951.0
52.00	202.0
52.90	112.0
55.00	230.0
56.00	1116.0
57.10	1859.0
60.00	742.0
61.00	3355.0
62.00	3402.0
63.00	2939.0
64.00	368.0
65.00	631.0
67.00	197.0
68.10	7236.0
69.00	7389.0
70.00	534.0
72.00	403.0
73.00	3391.0
74.00	11617.0
75.00	35008.0
76.00	2873.0
77.00	507.0
78.00	274.0
79.00	2775.0
79.90	876.0
80.90	2405.0
82.00	617.0
87.00	2767.0
88.00	2891.0
90.90	264.0
92.00	2120.0
93.00	2883.0
94.00	8845.0
95.00	68584.0
96.10	4779.0
97.00	193.0
103.90	341.0
104.90	106.0
105.90	352.0
106.90	128.0
110.70	118.0
112.80	110.0
115.90	347.0
116.90	537.0
117.90	288.0
118.90	526.0
127.90	270.0
129.00	139.0
130.00	290.0
130.90	141.0
134.80	169.0
137.00	144.0
141.00	838.0
142.00	116.0
142.90	992.0
143.80	110.0
145.00	343.0
145.80	151.0
148.00	210.0
149.80	110.0
154.90	225.0
170.60	107.0
172.00	696.0
173.00	753.0
174.00	58584.0
175.00	4389.0
176.00	56960.0
177.00	3743.0
177.90	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232

m/z	Abundance
36.00	639.0
37.10	3571.0
38.10	2850.0
39.00	1428.0
40.00	130.0
44.00	649.0
45.00	584.0
47.00	767.0
48.00	563.0
49.10	3028.0
50.10	13713.0
51.10	4269.0
52.00	227.0
52.90	131.0
55.00	288.0
56.00	1216.0
57.10	2050.0
60.00	794.0
61.00	3585.0
62.00	3653.0
63.00	3241.0
64.00	431.0
65.00	675.0
65.90	111.0
67.10	210.0
68.00	7576.0
69.00	7931.0
70.00	580.0
72.00	450.0
73.00	3602.0
74.10	12832.0
75.00	38760.0
76.00	3052.0
77.00	600.0
78.10	362.0
79.00	2900.0
79.90	943.0
80.90	2711.0
82.00	736.0
86.00	126.0
87.00	3004.0
88.00	3255.0
90.90	361.0
92.00	2349.0
93.00	3308.0
94.00	9522.0
95.00	75680.0
96.00	5304.0
97.00	218.0
103.90	352.0
104.90	123.0
105.90	405.0
106.90	130.0
110.70	146.0
112.90	106.0
115.00	110.0
115.90	346.0
116.80	558.0
118.00	314.0
118.90	591.0
128.00	332.0
128.90	134.0
130.00	352.0
130.90	144.0
134.90	193.0
136.90	162.0
141.00	904.0
142.00	125.0
143.00	1113.0
145.00	276.0
145.80	178.0
148.00	247.0
149.80	130.0
154.90	277.0
157.10	123.0
158.80	127.0
170.60	105.0
172.00	836.0
172.90	816.0
174.00	66320.0
175.00	5039.0
176.00	63984.0
177.00	4351.0
177.90	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232

m/z	Abundance
36.00	658.0
37.10	3578.0
38.10	2933.0
39.00	1360.0
39.90	136.0
44.00	613.0
45.10	569.0
47.00	757.0
48.00	605.0
49.10	2886.0
50.10	14139.0
51.10	4298.0
52.00	253.0
52.80	131.0
55.10	300.0
56.00	1272.0
57.10	2041.0
60.00	762.0
61.00	3572.0
62.00	3721.0
63.00	3183.0
64.00	428.0
65.00	679.0
65.90	124.0
67.10	214.0
68.00	7043.0
69.00	7677.0
70.00	596.0
72.00	448.0
73.00	3523.0
74.10	13150.0
75.00	38152.0
76.10	3124.0
77.00	585.0
78.10	384.0
78.90	2756.0
80.00	896.0
80.90	2797.0
82.00	732.0
85.90	163.0
86.90	3048.0
88.00	3374.0
90.90	420.0
92.00	2412.0
93.00	3526.0
94.00	9374.0
95.00	75064.0
96.10	5087.0
97.00	183.0
103.90	366.0
105.00	123.0
105.90	428.0
110.70	135.0
114.90	127.0
115.90	348.0
116.80	552.0
118.00	305.0
118.90	630.0
128.00	382.0
128.80	118.0
129.90	376.0
130.90	123.0
134.90	191.0
136.90	161.0
141.00	901.0
141.80	139.0
142.90	1122.0
145.00	197.0
145.80	187.0
147.10	106.0
148.00	221.0
149.80	129.0
154.90	289.0
157.10	126.0
158.80	162.0
160.80	104.0
172.00	881.0
173.00	788.0
174.00	67640.0
175.00	5190.0
176.00	65272.0
177.00	4471.0
178.00	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB232