

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111022\
 Data File : VV028869.D
 Acq On : 10 Nov 2022 15:08
 Operator : SY/MD
 Sample : N5574-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 B0AA1

Quant Time: Nov 11 02:06:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111022.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Nov 11 02:00:02 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.639	114	20268	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.863	117	18499	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.244	152	8780	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.310	65	10257	0.532	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	106.000%
4) 1,2-Dichloroethane-d4	5.042	65	6202	0.526	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	106.000%
7) 1,2-Dichloropropane-d6	6.068	67	8156	0.539	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	108.000%
8) Toluene-d8	7.317	98	22449	0.527	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	106.000%
10) 1,1,2,2-Tetrachloroeth...	10.198	84	4952	0.506	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	102.000%
Target Compounds						
						Qvalue
3) Vinyl chloride	1.310	62	237	0.013	ug/L #	1
6) Trichloroethene	5.925	95	162	0.012	ug/L #	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111022\
Data File : VV028869.D
Acq On : 10 Nov 2022 15:08
Operator : SY/MD
Sample : N5574-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
B0AA1

Quant Time: Nov 11 02:06:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111022.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Nov 11 02:00:02 2022
Response via : Initial Calibration

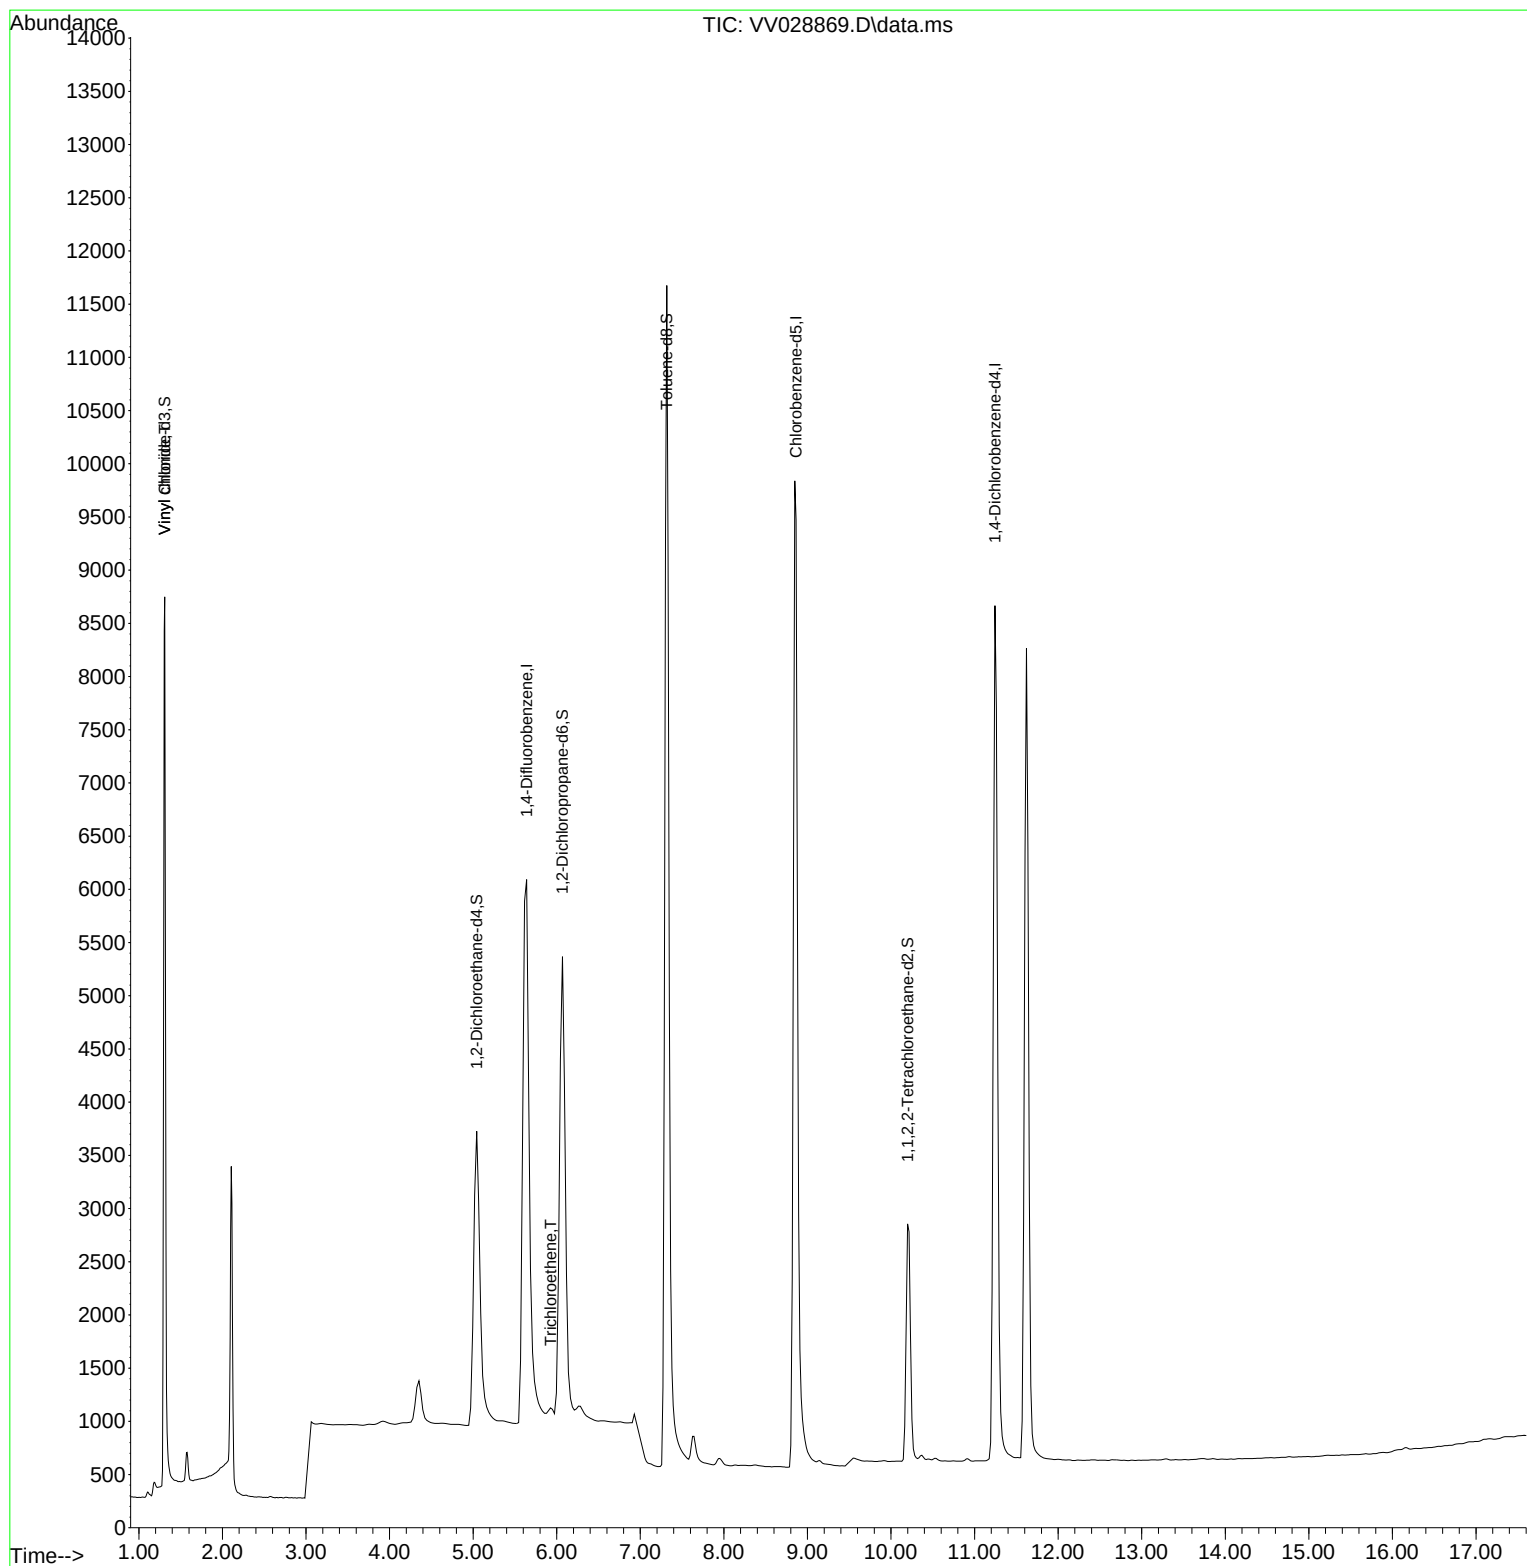

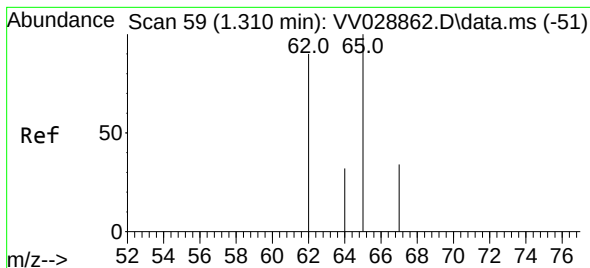

#3

Vinyl chloride

Concen: 0.013 ug/L

RT: 1.310 min Scan# 59

Delta R.T. 0.000 min

Lab File: VV028869.D

Acq: 10 Nov 2022 15:08

Instrument :

MSVOA_V

ClientSampleId :





B0AA1

Tgt Ion: 62 Resp: 237

Ion Ratio Lower Upper

62 100

64 153.0 26.8 49.8#

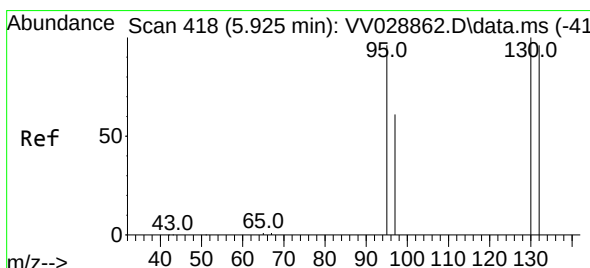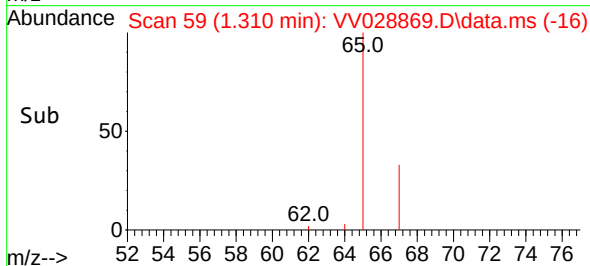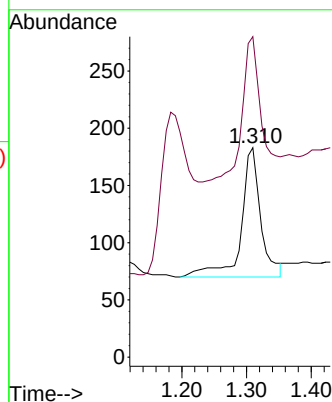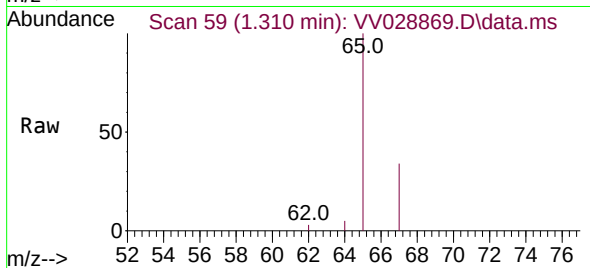

#6

Trichloroethene

Concen: 0.012 ug/L

RT: 5.925 min Scan# 418

Delta R.T. 0.000 min

Lab File: VV028869.D

Acq: 10 Nov 2022 15:08

Tgt Ion: 95 Resp: 162

Ion Ratio Lower Upper

95 100

97 88.8 45.8 85.0#

132 92.1 69.9 129.9

130 92.1 72.7 134.9

