
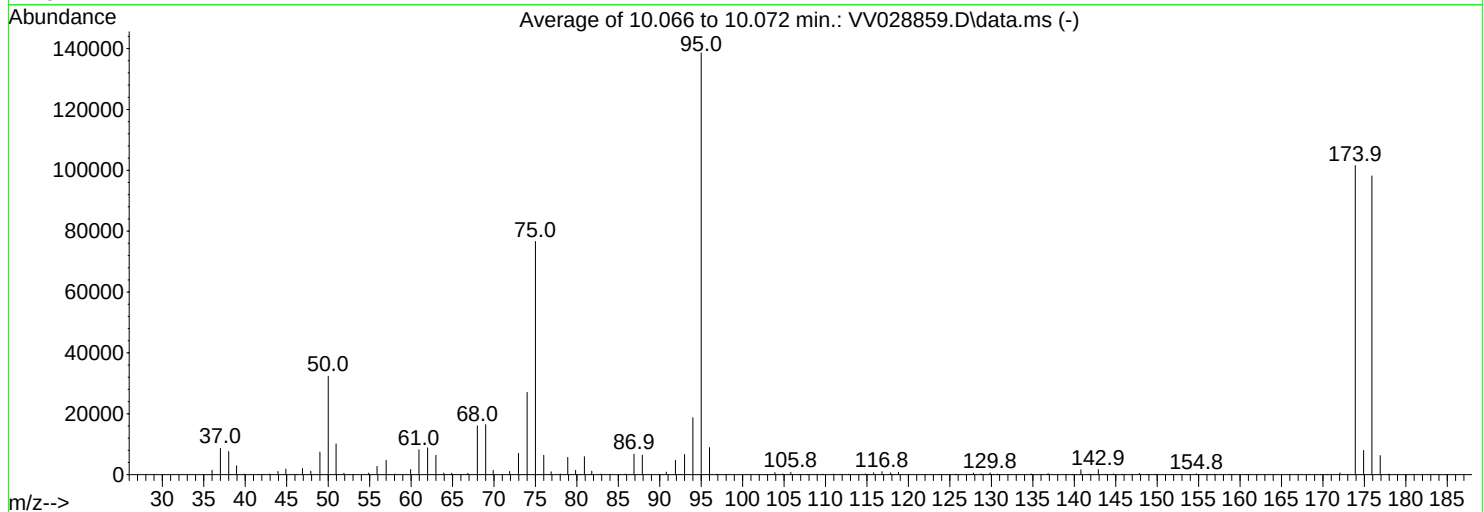


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111022\
 Data File : VV028859.D
 Acq On : 10 Nov 2022 09:16
 Operator : SY/MD
 Sample : BFB210
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB210

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM111022.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Nov 11 02:00:02 2022

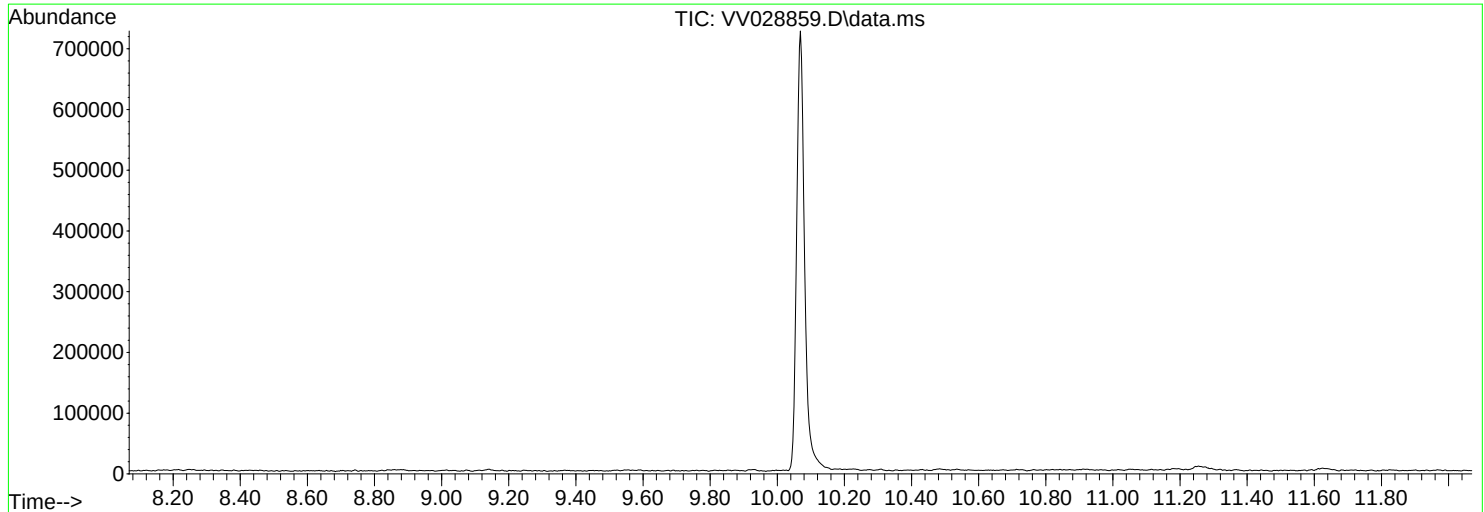

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.3	32352	PASS
75	95	30	80	55.3	76594	PASS
95	95	100	100	100.0	138603	PASS
96	95	5	9	6.4	8896	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.3	101563	PASS
175	174	5	9	7.8	7942	PASS
176	174	95	101	96.7	98165	PASS
177	176	5	9	6.4	6277	PASS

m/z	Abundance
35.60	210.0
36.60	126.0
37.20	151.0
37.70	126.0
38.80	210.0
39.90	521.0
40.70	189.0
41.20	139.0
42.00	156.0
42.80	107.0
43.90	984.0
45.90	128.0
46.40	152.0
47.60	147.0
48.00	104.0
48.70	124.0
49.60	108.0
50.30	121.0
50.80	121.0
53.00	116.0
53.60	132.0
54.90	115.0
55.30	110.0
56.70	131.0
58.50	107.0
60.40	164.0
63.50	120.0
67.70	145.0
68.40	116.0
69.90	119.0
75.20	107.0
81.50	139.0
85.00	110.0
88.40	104.0
96.80	143.0
107.20	101.0
121.70	111.0
132.70	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210

m/z	Abundance
36.00	1506.0
37.00	8926.0
38.00	7801.0
39.00	3151.0
39.90	728.0
40.90	147.0
41.60	103.0
43.00	324.0
44.00	1962.0
44.90	1860.0
45.80	135.0
46.90	2079.0
47.90	1253.0
49.00	7392.0
50.00	32576.0
51.00	10523.0
51.90	564.0
53.00	163.0
54.90	673.0
55.90	2772.0
57.00	4712.0
58.00	232.0
59.90	1611.0
61.00	8422.0
62.00	9056.0
63.00	6349.0
64.00	556.0
64.90	490.0
66.00	102.0
66.90	490.0
68.00	16016.0
69.00	16328.0
70.00	1574.0
71.90	1008.0
73.00	7055.0
74.00	27448.0
75.00	76856.0
76.00	6244.0
76.90	1003.0
78.90	5876.0
79.90	1432.0
80.90	5944.0
81.80	1153.0
82.90	263.0
85.90	256.0
86.90	7009.0
87.90	6266.0
90.00	110.0
90.80	880.0
91.90	4653.0
93.00	6620.0
94.00	18464.0
95.00	138752.0
96.00	8965.0
96.90	305.0
97.90	127.0
102.70	131.0
103.90	615.0
104.80	231.0
105.80	746.0
106.70	206.0
108.90	113.0
109.70	148.0
110.90	203.0
111.70	147.0
112.80	196.0
114.80	263.0
115.80	708.0
116.80	996.0
117.90	537.0
118.80	833.0
122.00	123.0
123.90	120.0
124.60	101.0
125.70	143.0
127.80	522.0
128.80	331.0
129.80	649.0
130.70	238.0
134.80	270.0
136.90	340.0
139.00	111.0
140.80	1558.0
141.80	248.0
142.90	1667.0
143.70	145.0
144.80	253.0
145.80	193.0
146.90	202.0
147.80	467.0
148.80	166.0
149.80	194.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210

151.80	107.0
152.80	138.0
154.70	268.0
155.70	116.0
156.90	151.0
158.80	161.0
160.70	131.0
169.00	108.0
170.60	153.0
172.00	547.0
173.90	99424.0
174.90	7910.0
175.90	95296.0
176.90	6381.0
177.90	195.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210

m/z	Abundance
36.00	1533.0
37.00	9073.0
38.00	7797.0
39.00	3212.0
39.90	717.0
40.80	154.0
41.60	103.0
43.00	316.0
44.00	2052.0
44.90	1893.0
46.20	163.0
46.90	2079.0
47.90	1318.0
49.00	7739.0
50.00	33456.0
51.00	10466.0
51.90	508.0
53.00	207.0
54.90	659.0
55.90	2811.0
57.00	4884.0
58.10	229.0
60.00	1743.0
60.90	8524.0
62.00	9178.0
63.00	6611.0
64.00	524.0
64.90	499.0
66.90	493.0
68.00	16592.0
69.00	17176.0
70.00	1596.0
71.90	1108.0
73.00	7195.0
74.00	27976.0
75.00	79240.0
76.00	6574.0
76.90	985.0
78.90	5840.0
79.90	1464.0
80.90	6069.0
81.80	1200.0
82.90	249.0
85.90	236.0
86.90	6993.0
87.90	6657.0
90.80	895.0
91.90	4921.0
93.00	6865.0
94.00	19544.0
95.00	143872.0
96.00	9090.0
96.90	302.0
97.90	130.0
102.90	108.0
103.90	703.0
104.90	252.0
105.80	779.0
106.90	186.0
108.90	151.0
109.70	161.0
110.90	251.0
111.70	130.0
112.80	190.0
114.80	268.0
115.80	691.0
116.80	995.0
117.80	583.0
118.80	826.0
123.00	114.0
123.90	126.0
125.70	140.0
127.80	538.0
128.70	285.0
129.80	651.0
130.70	204.0
134.80	273.0
136.90	364.0
138.90	103.0
140.80	1624.0
141.90	214.0
142.90	1732.0
143.80	161.0
144.70	272.0
145.90	191.0
146.90	135.0
147.80	434.0
148.80	133.0
149.80	177.0
151.80	122.0
152.80	137.0
153.80	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210

154.70	311.0
155.70	128.0
157.00	177.0
158.80	167.0
160.80	131.0
169.00	127.0
169.70	117.0
172.00	610.0
173.90	104760.0
174.90	8147.0
175.90	101704.0
176.90	6454.0
177.90	230.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210

m/z	Abundance
36.00	1467.0
37.00	8350.0
38.00	7119.0
39.00	2989.0
39.90	699.0
40.80	156.0
41.40	121.0
42.20	106.0
43.00	298.0
44.00	2097.0
44.90	1727.0
46.10	190.0
46.90	1893.0
47.90	1223.0
49.00	7192.0
50.00	31024.0
51.00	9626.0
51.90	438.0
53.00	195.0
54.90	575.0
55.90	2573.0
57.00	4557.0
58.10	214.0
58.60	106.0
60.00	1684.0
60.90	7733.0
62.00	8196.0
63.00	6143.0
63.90	509.0
64.90	491.0
66.80	463.0
68.00	15540.0
69.00	15885.0
69.90	1418.0
70.90	136.0
71.90	1024.0
72.90	6656.0
74.00	25680.0
75.00	74008.0
76.00	6252.0
76.90	913.0
78.00	693.0
78.90	5346.0
79.80	1436.0
80.90	5592.0
81.80	1149.0
82.90	196.0
85.90	171.0
86.90	6226.0
87.90	6416.0
90.80	720.0
91.90	4590.0
93.00	6338.0
94.00	18160.0
95.00	133184.0
96.00	8634.0
96.90	292.0
97.80	132.0
103.00	122.0
103.90	787.0
104.90	305.0
105.80	727.0
107.00	209.0
107.80	131.0
109.00	131.0
109.70	151.0
111.00	236.0
111.80	127.0
112.80	172.0
114.80	226.0
115.80	579.0
116.80	960.0
117.80	616.0
118.80	763.0
123.00	121.0
123.90	104.0
125.70	125.0
127.90	574.0
128.70	217.0
129.90	510.0
130.80	184.0
134.80	321.0
136.80	352.0
139.80	148.0
140.80	1504.0
142.90	1641.0
143.80	165.0
144.70	222.0
145.70	173.0
147.90	393.0
149.90	152.0
151.80	133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210

152.80	106.0
153.80	124.0
154.80	354.0
155.80	120.0
156.80	187.0
158.80	182.0
160.80	125.0
169.00	118.0
169.70	147.0
170.50	155.0
172.10	537.0
173.90	100504.0
174.90	7769.0
175.90	97496.0
176.90	5996.0
178.00	219.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210