

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111023\
 Data File : VW032883.D
 Acq On : 10 Nov 2023 11:47
 Operator : SY/MD
 Sample : 05333-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGD5

Quant Time: Nov 10 22:50:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 08 01:37:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	317376	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	348183	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	156899	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	115625	38.303	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	76.600%		
7) Chloroethane-d5	1.532	69	103159	40.860	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	81.720%		
11) 1,1-Dichloroethene-d2	2.060	65	51253	41.106	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.220%		
21) 2-Butanone-d5	3.786	46	114929	87.775	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	87.780%		
24) Chloroform-d	4.252	84	208253	43.221	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.440%		
26) 1,2-Dichloroethane-d4	4.944	65	136344	45.530	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.060%		
32) Benzene-d6	4.963	84	401497	44.848	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.700%		
36) 1,2-Dichloropropane-d6	5.989	67	134296	49.378	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	98.760%		
41) Toluene-d8	7.246	98	379997	43.108	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.220%		
43) trans-1,3-Dichloroprop...	7.555	79	60006	42.363	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.720%		
47) 2-Hexanone-d5	8.027	63	77986	78.543	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	78.540%		
56) 1,1,2,2-Tetrachloroeth...	10.156	84	177299	42.959	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	85.920%		
66) 1,2-Dichlorobenzene-d4	11.564	152	156821	51.867	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	103.740%		
Target Compounds					Qvalue	
13) Acetone	2.114	43	17603	8.032	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032883.D
Acq On : 10 Nov 2023 11:47
Operator : SY/MD
Sample : 05333-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGD5

Quant Time: Nov 10 22:50:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 08 01:37:19 2023
Response via : Initial Calibration

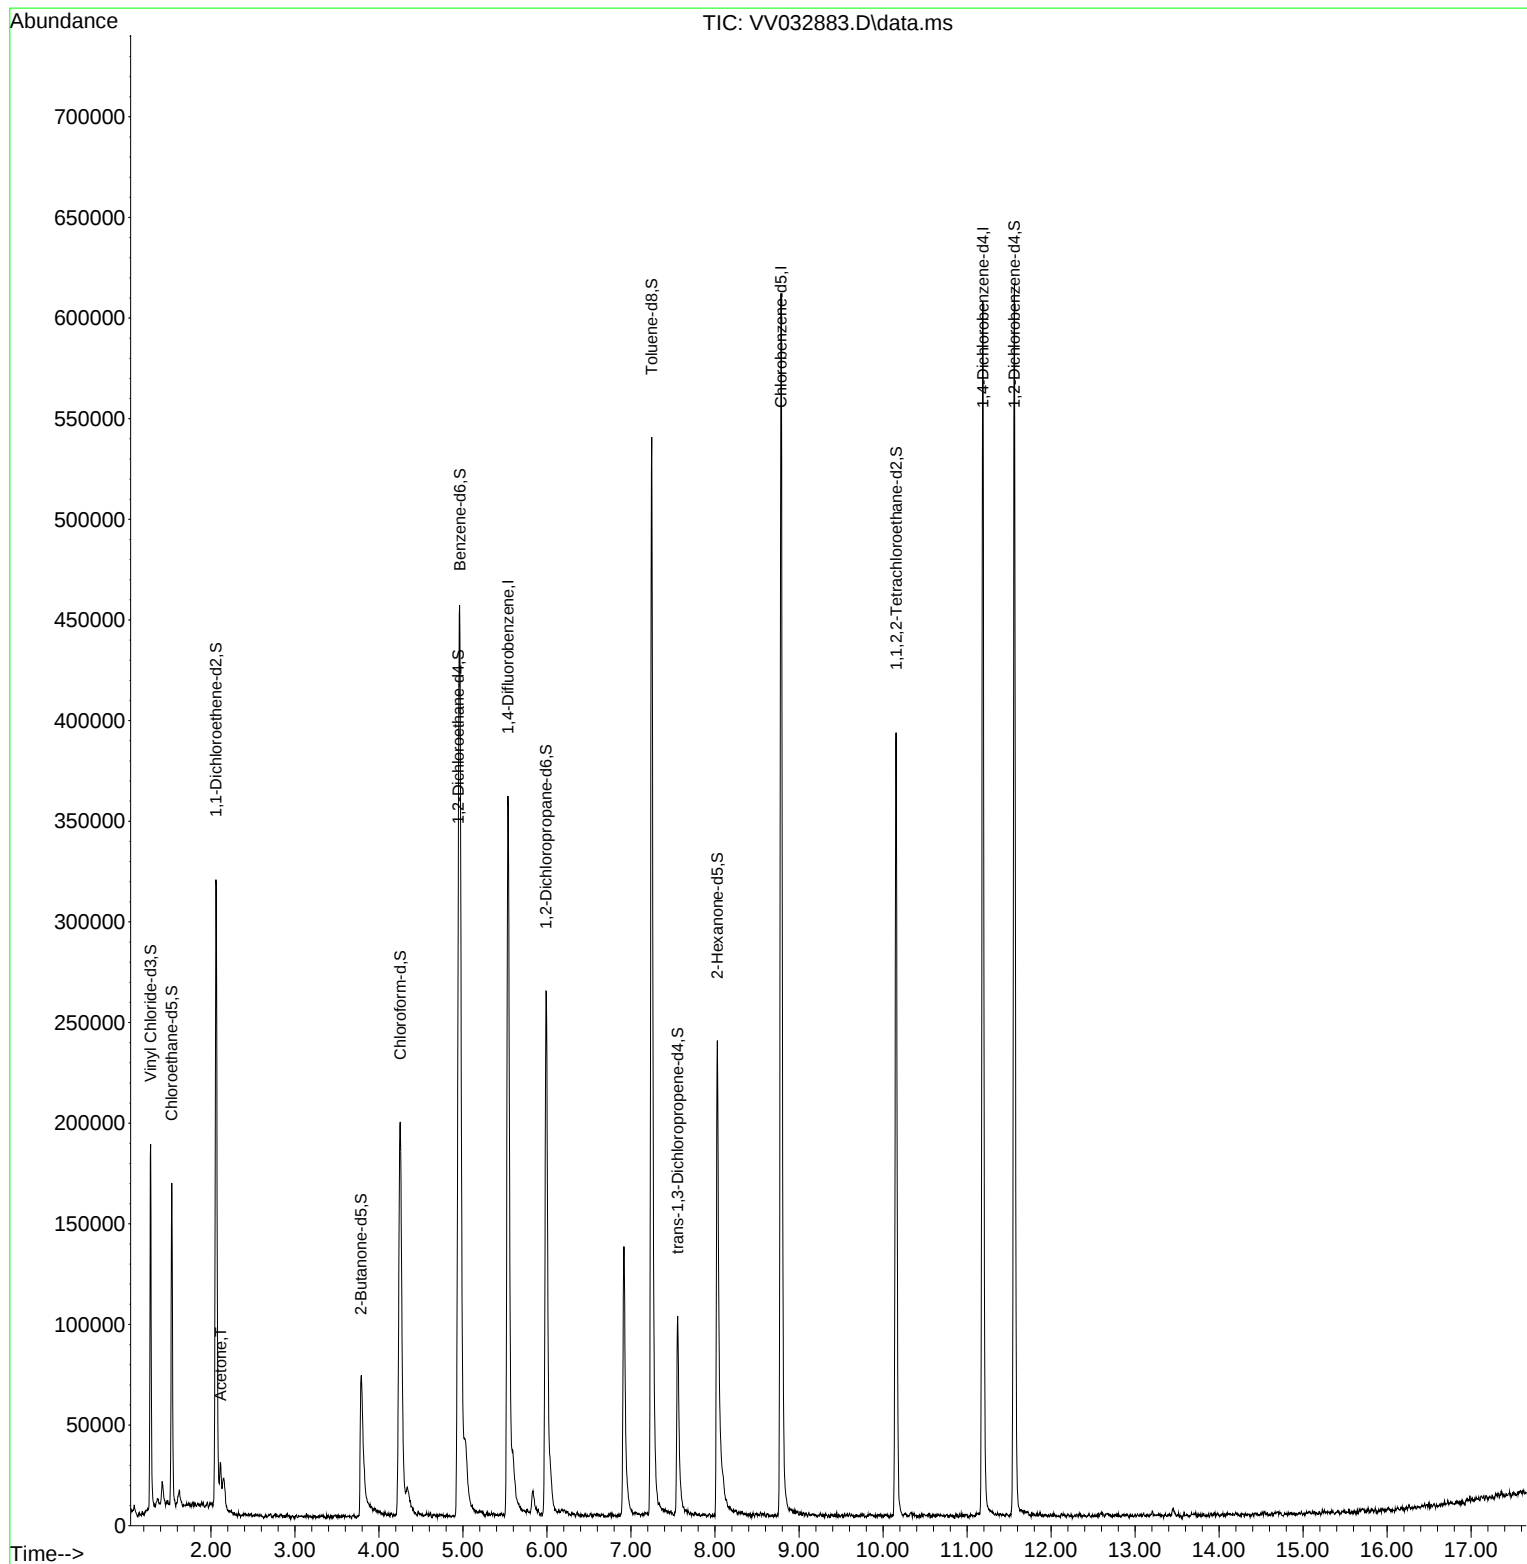

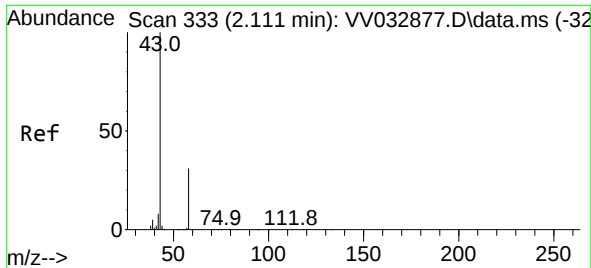

#13
 Acetone
 Concen: 8.032 ug/L
 RT: 2.114 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV032883.D
 Acq: 10 Nov 2023 11:47

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGD5

Tgt Ion: 43 Resp: 17603
 Ion Ratio Lower Upper
 43 100
 58 35.1 0.0 61.2

