

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111023\
 Data File : VW032899.D
 Acq On : 10 Nov 2023 18:03
 Operator : SY/MD
 Sample : 05296-16 10X
 Misc : 5.45gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3T2

Quant Time: Nov 10 22:52:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 08 01:37:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	383270	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	389205	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	182820	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	125067	34.308	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	68.620%		
7) Chloroethane-d5	1.523	69	120870	39.645	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	79.280%		
11) 1,1-Dichloroethene-d2	2.056	65	59460	39.490	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	78.980%		
21) 2-Butanone-d5	3.786	46	130040	82.241	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	82.240%		
24) Chloroform-d	4.249	84	250408	43.035	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.080%		
26) 1,2-Dichloroethane-d4	4.941	65	169468	46.861	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.720%		
32) Benzene-d6	4.960	84	505359	50.500	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	101.000%		
36) 1,2-Dichloropropane-d6	5.989	67	153840	50.602	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	101.200%		
41) Toluene-d8	7.246	98	439644	44.618	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	89.240%		
43) trans-1,3-Dichloroprop...	7.555	79	71797	45.345	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	90.680%		
47) 2-Hexanone-d5	8.027	63	95390	85.945	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	85.950%		
56) 1,1,2,2-Tetrachloroeth...	10.156	84	209026	45.308	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	90.620%		
66) 1,2-Dichlorobenzene-d4	11.561	152	188023	53.369	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	106.740%		
Target Compounds						Qvalue
46) Tetrachloroethene	7.911	164	2304	0.889	ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032899.D
Acq On : 10 Nov 2023 18:03
Operator : SY/MD
Sample : 05296-16 10X
Misc : 5.45gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3T2


Quant Time: Nov 10 22:52:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 08 01:37:19 2023
Response via : Initial Calibration

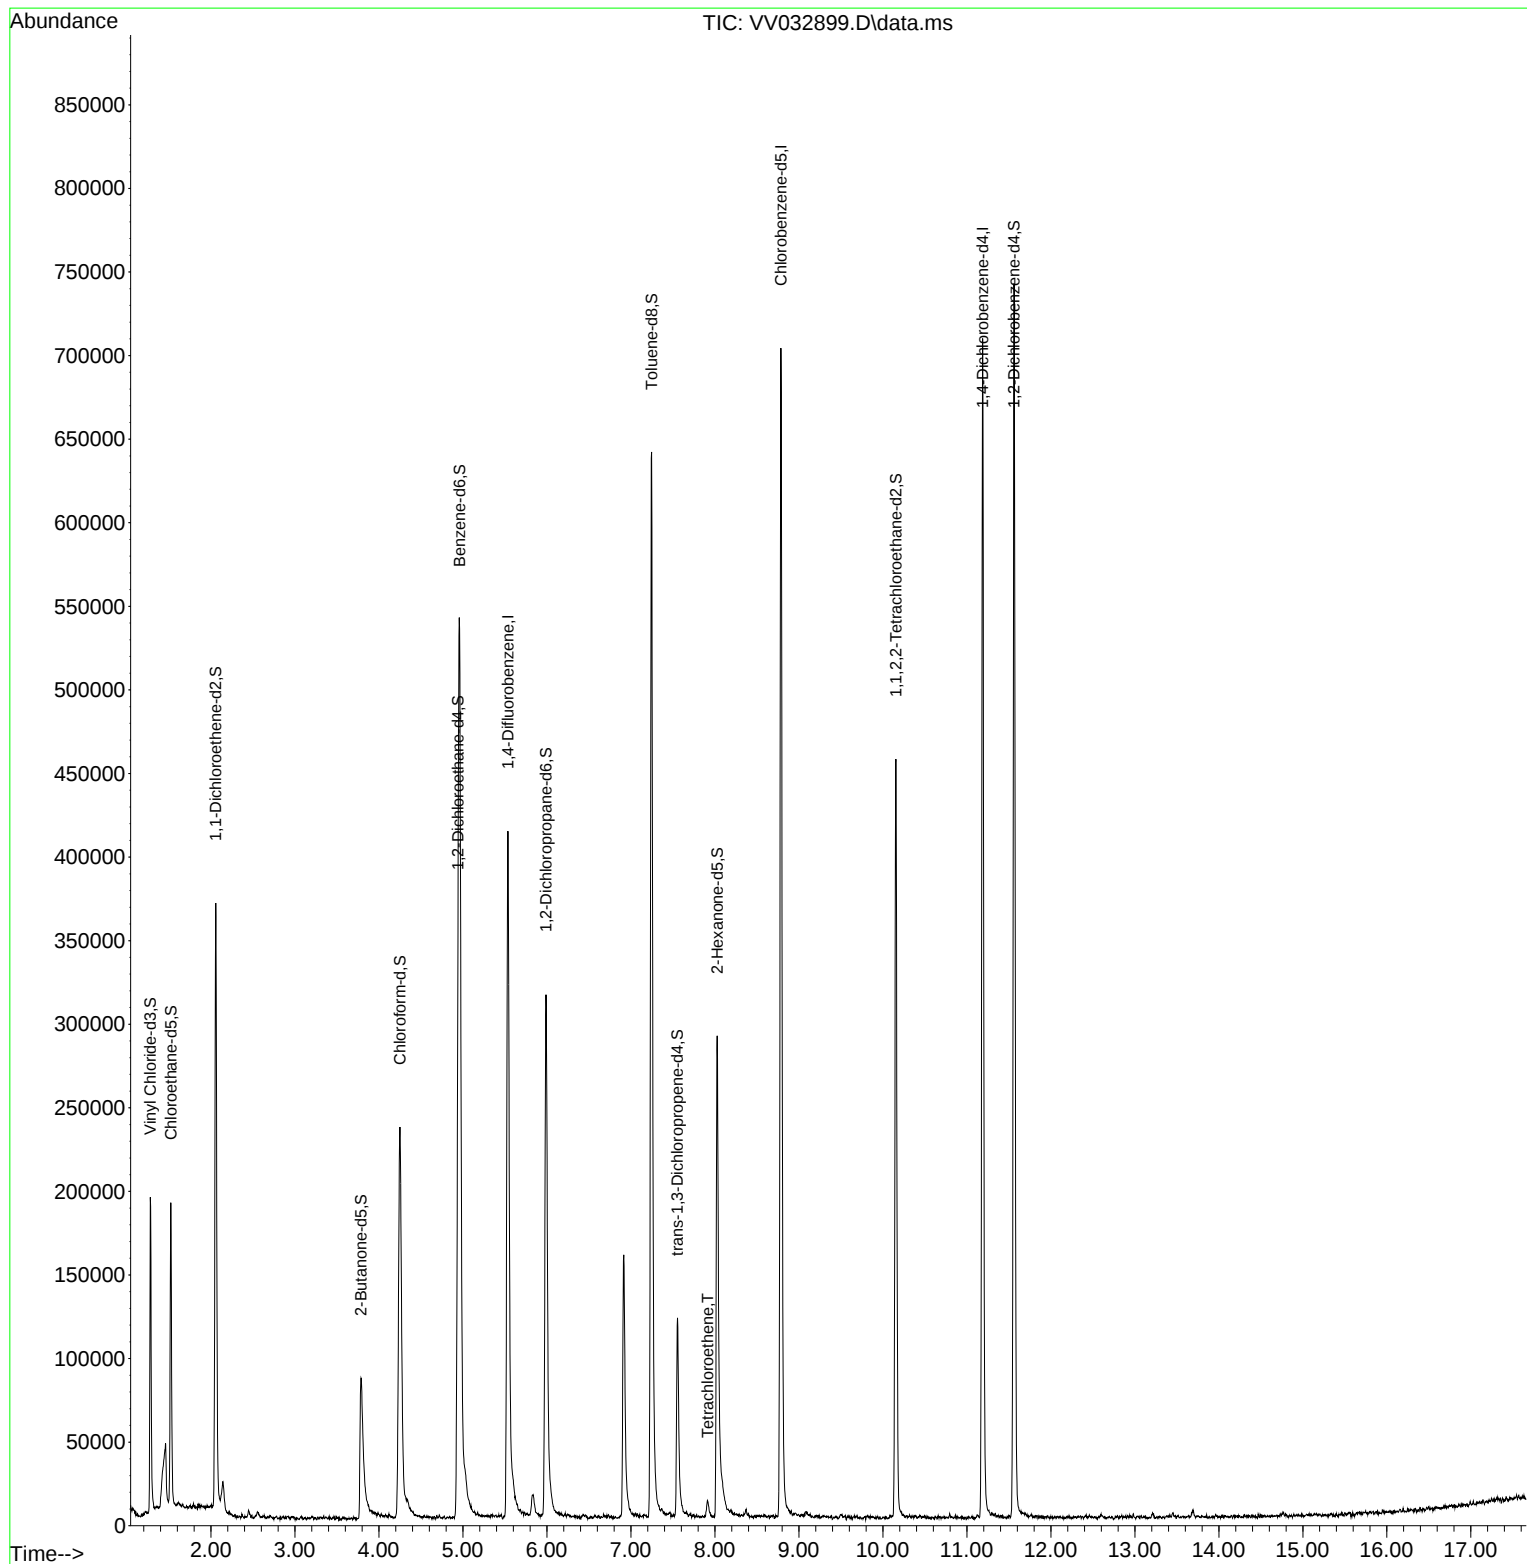

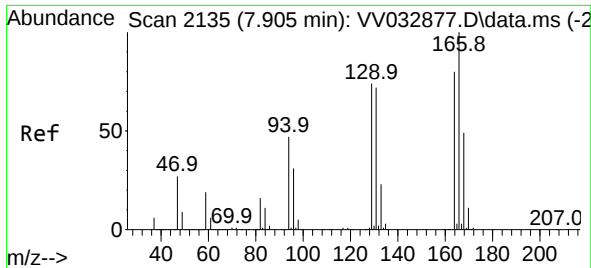

#46
 Tetrachloroethene
 Concen: 0.889 ug/L
 RT: 7.911 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VV032899.D
 Acq: 10 Nov 2023 18:03

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3T2

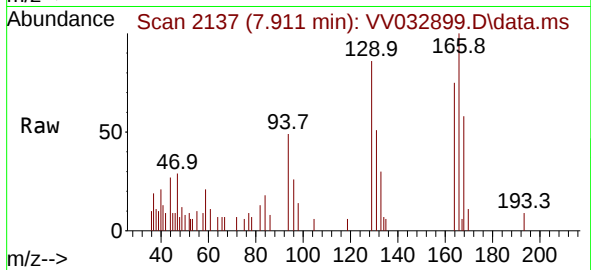

Tgt Ion:	164	Resp:	2304
Ion	Ratio	Lower	Upper
164	100		
129	115.5	65.3	121.3
131	68.1	65.0	120.8
166	133.6	87.8	163.2

