

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032903.D
 Acq On : 10 Nov 2023 20:23
 Operator : SY/MD
 Sample : 05296-03 10X
 Misc : 5.03gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3R3

Quant Time: Nov 10 21:39:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 08 01:37:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	321662	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	327020	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	147827	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	102019	33.346	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	66.700%		
7) Chloroethane-d5	1.523	69	106438	41.597	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	83.200%		
11) 1,1-Dichloroethene-d2	2.056	65	49363	39.063	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	78.120%		
21) 2-Butanone-d5	3.786	46	130134	98.064	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	98.060%		
24) Chloroform-d	4.249	84	228402	46.771	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.540%		
26) 1,2-Dichloroethane-d4	4.941	65	153859	50.694	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	101.380%		
32) Benzene-d6	4.960	84	454987	54.112	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	108.220%		
36) 1,2-Dichloropropane-d6	5.989	67	143970	56.360	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	112.720%		
41) Toluene-d8	7.246	98	382468	46.196	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.400%		
43) trans-1,3-Dichloroprop...	7.555	79	65797	49.457	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	98.920%		
47) 2-Hexanone-d5	8.027	63	97559	104.614	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	104.610%		
56) 1,1,2,2-Tetrachloroeth...	10.156	84	201655	52.022	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	104.040%		
66) 1,2-Dichlorobenzene-d4	11.564	152	158586	55.669	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	111.340%		
Target Compounds						Qvalue
46) Tetrachloroethene	7.911	164	1393	0.640	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032903.D
Acq On : 10 Nov 2023 20:23
Operator : SY/MD
Sample : 05296-03 10X
Misc : 5.03gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3R3

Quant Time: Nov 10 21:39:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 08 01:37:19 2023
Response via : Initial Calibration

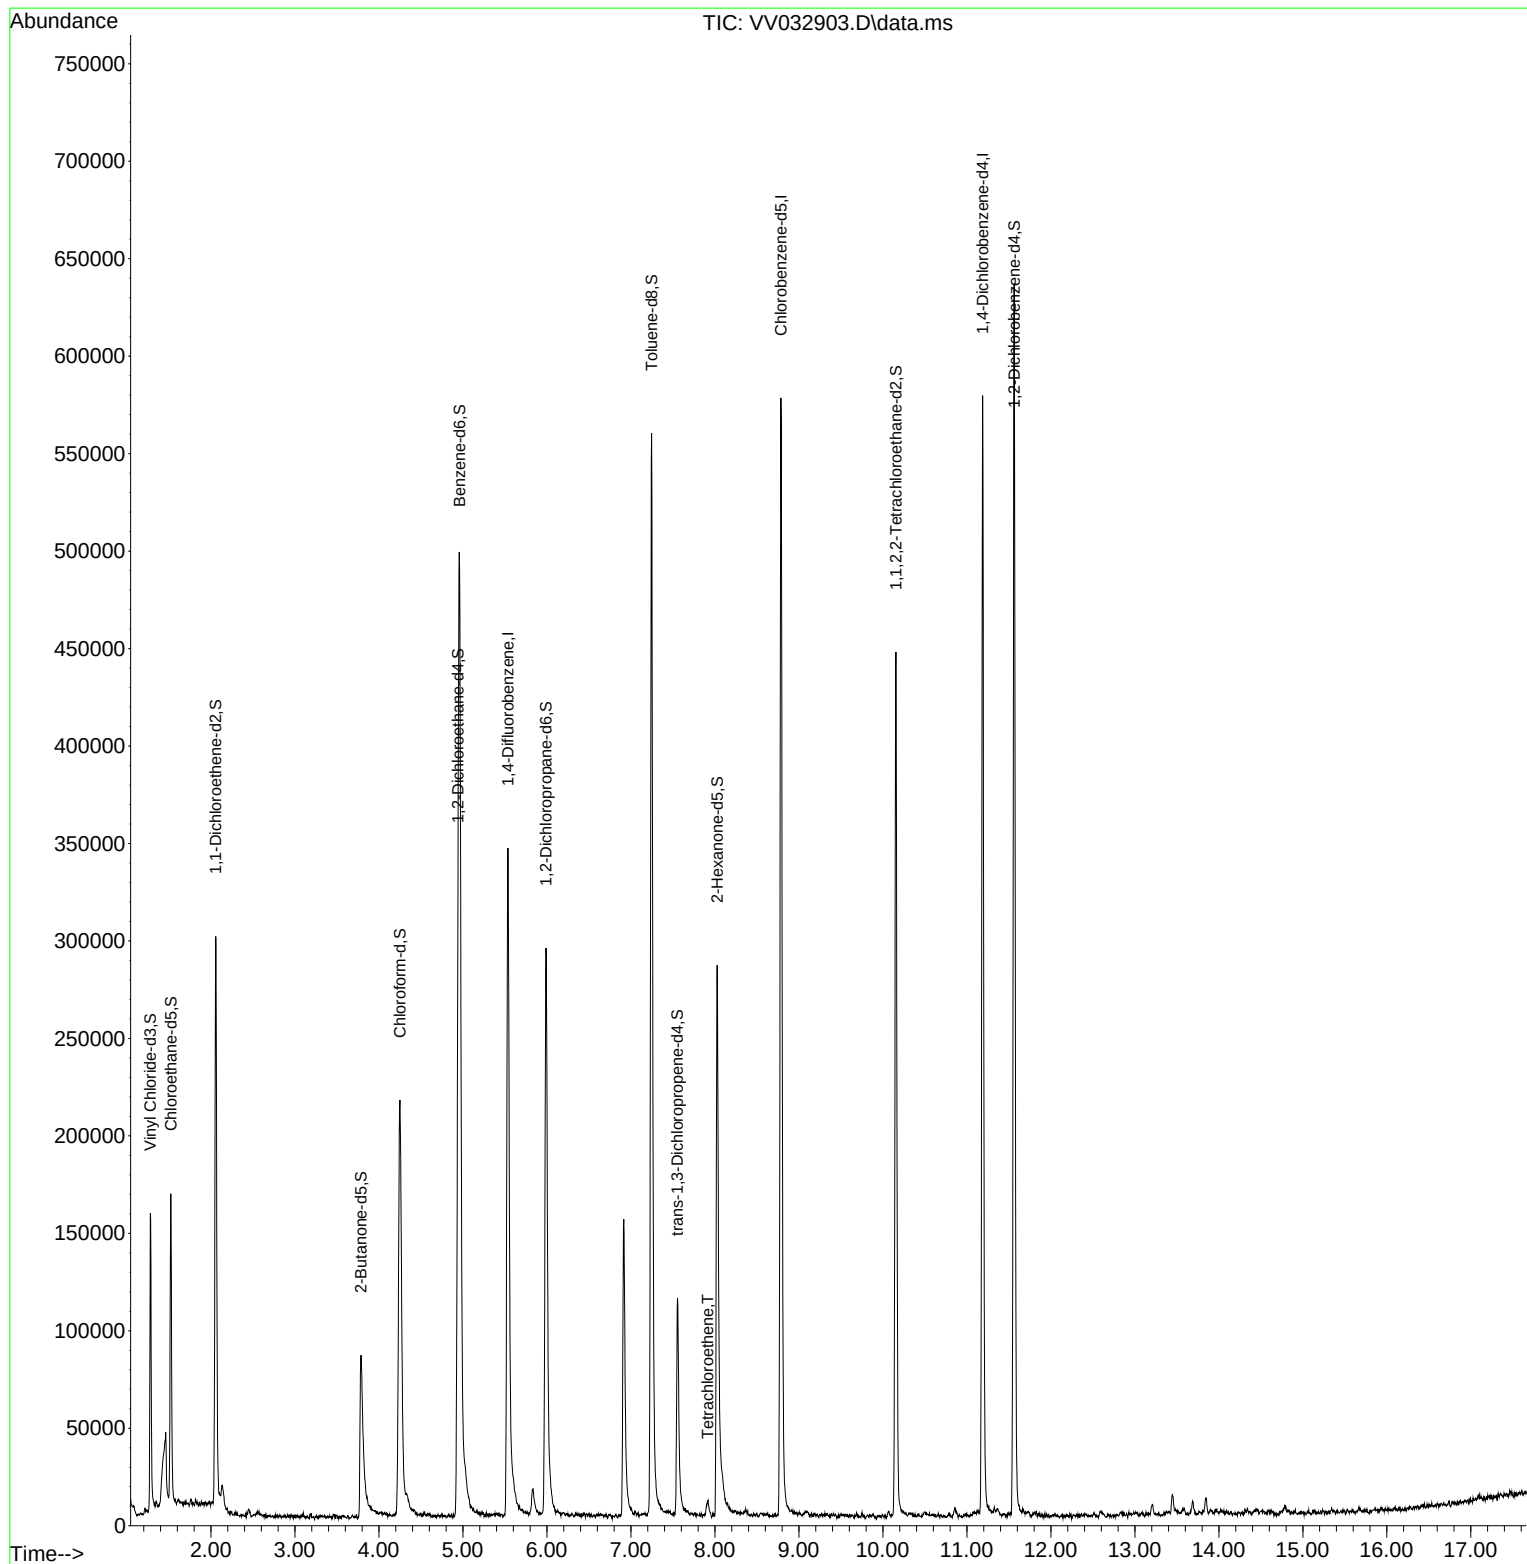

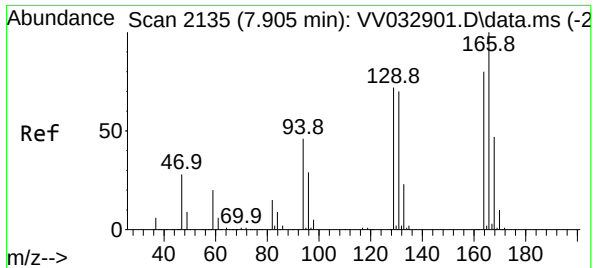

#46
 Tetrachloroethene
 Concen: 0.640 ug/L
 RT: 7.911 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VV032903.D
 Acq: 10 Nov 2023 20:23

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3R3

Tgt Ion:164 Resp: 1393

Ion	Ratio	Lower	Upper
164	100		
129	105.8	65.3	121.3
131	85.1	65.0	120.8
166	139.7	87.8	163.2

