

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032904.D
 Acq On : 10 Nov 2023 20:46
 Operator : SY/MD
 Sample : 05296-18 10X
 Misc : 5.53gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3T5

Quant Time: Nov 11 01:29:47 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 08 01:37:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	363759	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	369958	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	172849	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	123389	35.663	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	71.320%
7) Chloroethane-d5	1.523	69	120268	41.563	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	83.120%
11) 1,1-Dichloroethene-d2	2.056	65	57472	40.217	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.440%
21) 2-Butanone-d5	3.786	46	130324	86.842	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	86.840%
24) Chloroform-d	4.249	84	260484	47.168	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.340%
26) 1,2-Dichloroethane-d4	4.944	65	161276	46.988	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.980%
32) Benzene-d6	4.960	84	494607	51.997	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.000%
36) 1,2-Dichloropropane-d6	5.989	67	152129	52.642	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	105.280%
41) Toluene-d8	7.246	98	433386	46.271	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.540%
43) trans-1,3-Dichloroprop...	7.555	79	69047	45.876	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.760%
47) 2-Hexanone-d5	8.027	63	94334	89.416	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.420%
56) 1,1,2,2-Tetrachloroeth...	10.152	84	205337	46.824	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	93.640%
66) 1,2-Dichlorobenzene-d4	11.564	152	180547	54.203	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	108.400%
Target Compounds						
					Qvalue	
46) Tetrachloroethene	7.911	164	1446	0.587	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032904.D
Acq On : 10 Nov 2023 20:46
Operator : SY/MD
Sample : 05296-18 10X
Misc : 5.53gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3T5

Quant Time: Nov 11 01:29:47 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 08 01:37:19 2023
Response via : Initial Calibration

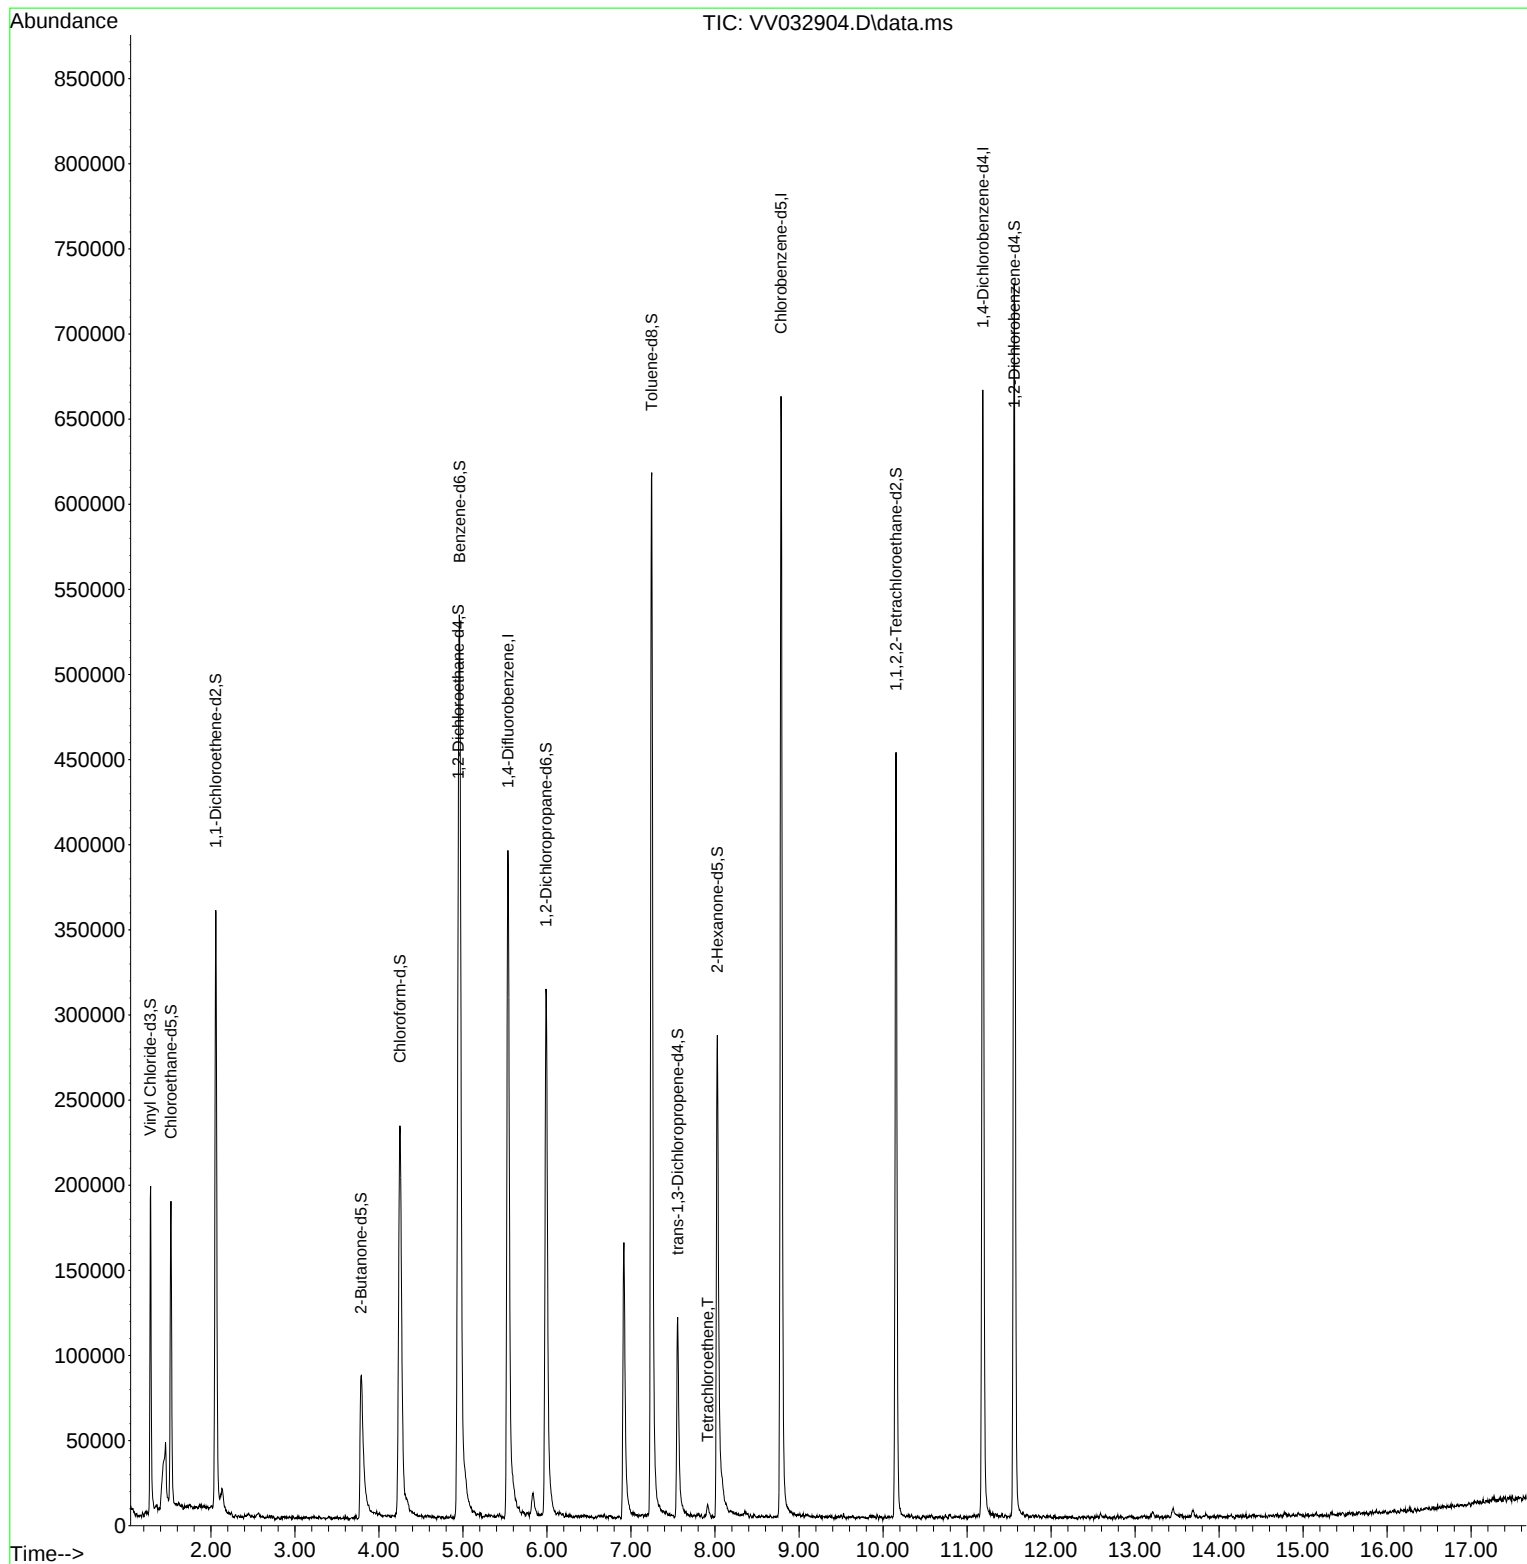

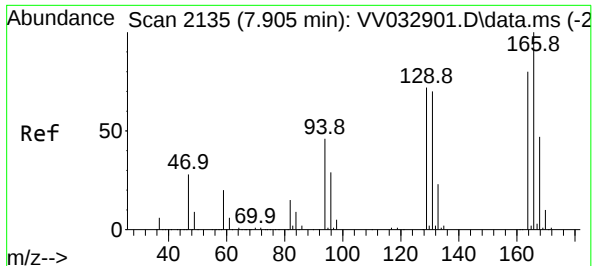

#46
 Tetrachloroethene
 Concen: 0.587 ug/L
 RT: 7.911 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VV032904.D
 Acq: 10 Nov 2023 20:46

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3T5

Tgt Ion:164 Resp: 1446

Ion	Ratio	Lower	Upper
164	100		
129	104.1	65.3	121.3
131	88.4	65.0	120.8
166	118.2	87.8	163.2

