

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111023\
 Data File : VW032905.D
 Acq On : 10 Nov 2023 21:09
 Operator : SY/MD
 Sample : 05296-20 10X
 Misc : 4.76gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3T8

Quant Time: Nov 11 01:30:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 08 01:37:19 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	368643	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	378457	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	176352	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	126039	35.947	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	71.900%		
7) Chloroethane-d5	1.523	69	119876	40.879	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	81.760%		
11) 1,1-Dichloroethene-d2	2.056	65	60015	41.440	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.880%		
21) 2-Butanone-d5	3.786	46	122819	80.756	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	80.760%		
24) Chloroform-d	4.249	84	246418	44.030	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.060%		
26) 1,2-Dichloroethane-d4	4.940	65	167429	48.134	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.260%		
32) Benzene-d6	4.960	84	498158	51.194	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.380%		
36) 1,2-Dichloropropane-d6	5.992	67	150107	50.776	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	101.560%		
41) Toluene-d8	7.246	98	439366	45.856	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.720%		
43) trans-1,3-Dichloroprop...	7.554	79	70861	46.024	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	92.040%		
47) 2-Hexanone-d5	8.027	63	92416	85.630	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	85.630%		
56) 1,1,2,2-Tetrachloroeth...	10.156	84	209074	46.605	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	93.220%		
66) 1,2-Dichlorobenzene-d4	11.564	152	183822	54.090	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	108.180%		
Target Compounds						Qvalue
46) Tetrachloroethene	7.915	164	1769	0.702	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032905.D
Acq On : 10 Nov 2023 21:09
Operator : SY/MD
Sample : 05296-20 10X
Misc : 4.76gm/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH3T8

Quant Time: Nov 11 01:30:04 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 08 01:37:19 2023
Response via : Initial Calibration

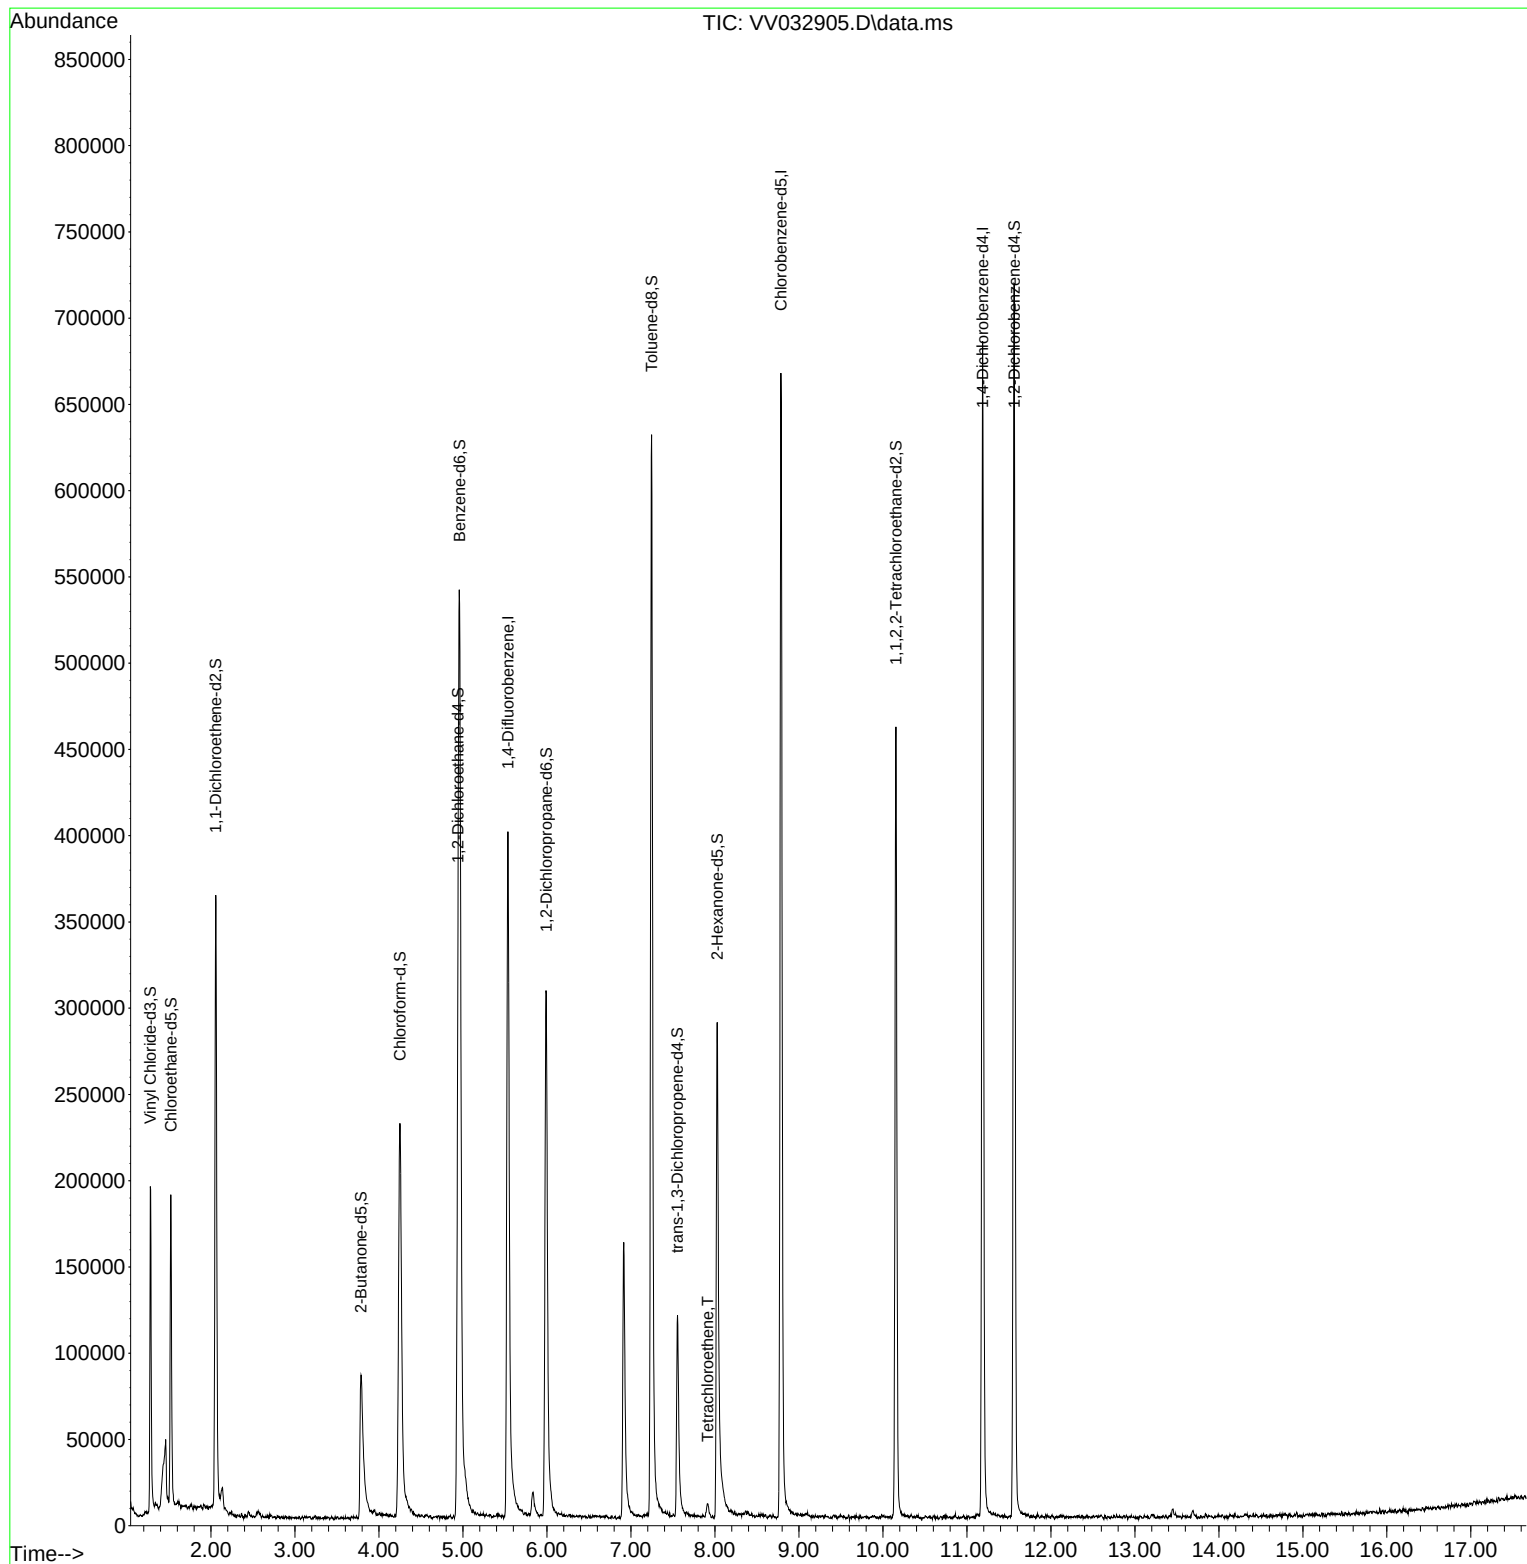

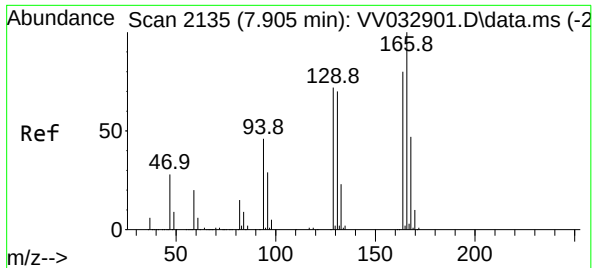

#46
 Tetrachloroethene
 Concen: 0.702 ug/L
 RT: 7.915 min Scan# 21
 Delta R.T. 0.010 min
 Lab File: VV032905.D
 Acq: 10 Nov 2023 21:09

Instrument :
 MSVOA_V
 ClientSampleId :
 BH3T8

Tgt Ion:164 Resp: 1769

Ion	Ratio	Lower	Upper
164	100		
129	116.8	65.3	121.3
131	91.9	65.0	120.8
166	120.3	87.8	163.2

