

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032879.D
 Acq On : 10 Nov 2023 10:03
 Operator : SY/MD
 Sample : VV1110WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK215

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032879.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	88	rBV	261776	266199	16.56%	2.131%
2	1.532	147	153	167	rVB	209865	246830	15.36%	1.976%
3	2.063	309	318	333	rBV	426697	611346	38.04%	4.893%
4	2.391	418	420	421	rBV2	1039	411	0.03%	0.003%
5	2.413	425	427	430	rVB4	1691	780	0.05%	0.006%
6	2.436	431	434	435	rBV3	1963	1229	0.08%	0.010%
7	2.622	490	492	494	rBV3	1134	807	0.05%	0.006%
8	2.664	503	505	508	rBV4	1714	890	0.06%	0.007%
9	2.764	534	536	537	rBV2	1155	564	0.04%	0.005%
10	2.796	544	546	549	rVB3	1596	735	0.05%	0.006%
11	2.818	551	553	556	rVB4	1941	1197	0.07%	0.010%
12	2.941	588	591	592	rBV2	1056	556	0.03%	0.004%
13	2.966	596	599	601	rBV4	1741	1287	0.08%	0.010%
14	3.076	631	633	634	rBV3	1447	604	0.04%	0.005%
15	3.137	650	652	654	rBV2	1610	579	0.04%	0.005%
16	3.217	674	677	679	rBV4	1294	925	0.06%	0.007%
17	3.285	694	698	700	rVB5	1509	1042	0.06%	0.008%
18	3.301	701	703	710	rVB7	1788	1297	0.08%	0.010%
19	3.330	710	712	715	rBV3	1160	779	0.05%	0.006%
20	3.384	727	729	733	rBV5	1109	765	0.05%	0.006%
21	3.400	733	734	737	rVB3	1638	560	0.03%	0.004%
22	3.429	737	743	746	rBV8	2590	2608	0.16%	0.021%
23	3.465	752	754	756	rVB3	913	425	0.03%	0.003%
24	3.484	756	760	762	rBV4	843	566	0.04%	0.005%
25	3.513	766	769	770	rVB2	1392	664	0.04%	0.005%
26	3.523	770	772	776	rVB5	1535	1034	0.06%	0.008%
27	3.545	776	779	781	rBV3	1891	1330	0.08%	0.011%
28	3.613	794	800	801	rBV6	1681	1107	0.07%	0.009%
29	3.719	831	833	837	rVB4	1087	664	0.04%	0.005%
30	3.738	837	839	840	rBV2	1709	719	0.04%	0.006%
31	3.786	845	854	883	rBV2	95377	265121	16.49%	2.122%
32	4.146	964	966	969	rBV3	1166	471	0.03%	0.004%
33	4.252	984	999	1018	rBV	257186	663184	41.26%	5.308%
34	4.529	1082	1085	1087	rBV4	1485	986	0.06%	0.008%
35	4.722	1142	1145	1146	rBV3	1776	888	0.06%	0.007%
36	4.960	1201	1219	1235	rBV2	605384	1607295	100.00%	12.864%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032879.D
 Acq On : 10 Nov 2023 10:03
 Operator : SY/MD
 Sample : VV1110WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK215

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	5.535	1387	1398	1414	rBV	407309	852212	53.02%	6.821%
38	5.989	1528	1539	1569	rBV2	339068	757348	47.12%	6.062%
39	6.285	1628	1631	1634	rBV5	1659	944	0.06%	0.008%
40	6.416	1670	1672	1674	rBV3	1674	760	0.05%	0.006%
41	6.757	1775	1778	1782	rBV6	2227	1763	0.11%	0.014%
42	6.915	1817	1827	1854	rBV	183051	371986	23.14%	2.977%
43	7.243	1919	1929	1959	rBV	736150	1381958	85.98%	11.061%
44	7.555	2017	2026	2047	rBV	134993	249601	15.53%	1.998%
45	7.902	2132	2134	2135	rVB2	1740	420	0.03%	0.003%
46	8.027	2163	2173	2203	rBV	328560	674172	41.94%	5.396%
47	8.458	2304	2307	2310	rBV5	1744	1245	0.08%	0.010%
48	8.667	2369	2372	2375	rBV5	1684	1589	0.10%	0.013%
49	8.786	2396	2409	2437	rBV	702698	1194552	74.32%	9.561%
50	9.400	2597	2600	2603	rBV4	1358	1042	0.06%	0.008%
51	9.426	2606	2608	2610	rVV3	1992	981	0.06%	0.008%
52	9.439	2610	2612	2614	rVB2	2143	950	0.06%	0.008%
53	9.580	2654	2656	2659	rBV4	2200	1628	0.10%	0.013%
54	9.686	2686	2689	2691	rBV4	1193	868	0.05%	0.007%
55	9.722	2697	2700	2703	rBV5	1631	1343	0.08%	0.011%
56	9.764	2711	2713	2715	rBV3	1097	640	0.04%	0.005%
57	9.802	2720	2725	2727	rBV6	1957	1792	0.11%	0.014%
58	9.863	2741	2744	2745	rBV3	2289	1089	0.07%	0.009%
59	9.947	2766	2770	2771	rBV4	1220	754	0.05%	0.006%
60	10.037	2795	2798	2804	rVB8	1804	1965	0.12%	0.016%
61	10.066	2804	2807	2812	rBV6	2162	2123	0.13%	0.017%
62	10.104	2815	2819	2823	rBV6	2089	2329	0.14%	0.019%
63	10.156	2823	2835	2854	rBV	501270	808777	50.32%	6.473%
64	10.535	2951	2953	2954	rBV2	858	400	0.02%	0.003%
65	10.612	2975	2977	2983	rVB6	2561	2047	0.13%	0.016%
66	10.654	2984	2990	2993	rBV6	1809	2133	0.13%	0.017%
67	10.709	3004	3007	3008	rBV3	1381	649	0.04%	0.005%
68	10.828	3039	3044	3049	rVB8	2108	2074	0.13%	0.017%
69	10.969	3087	3088	3090	rBV2	1057	399	0.02%	0.003%
70	10.982	3090	3092	3094	rVV3	1169	384	0.02%	0.003%
71	11.024	3102	3105	3107	rBV3	1434	879	0.05%	0.007%
72	11.114	3131	3133	3135	rBV3	2517	1427	0.09%	0.011%
73	11.188	3145	3156	3180	rVB	712208	1110581	69.10%	8.889%
74	11.471	3243	3244	3245	rBV	1284	449	0.03%	0.004%
75	11.561	3260	3272	3298	rBV	814280	1297460	80.72%	10.385%
76	11.979	3400	3402	3405	rBV4	1580	814	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032879.D
 Acq On : 10 Nov 2023 10:03
 Operator : SY/MD
 Sample : VV1110WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK215

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	12.088	3434	3436	3438	rBV3	1504	1065	0.07%	0.009%
78	12.207	3471	3473	3478	rVB5	1082	594	0.04%	0.005%
79	12.243	3482	3484	3488	rVB4	2614	1537	0.10%	0.012%
80	12.268	3490	3492	3493	rBV2	1389	706	0.04%	0.006%
81	12.304	3500	3503	3504	rBV3	976	523	0.03%	0.004%
82	12.345	3514	3516	3519	rBV4	1680	923	0.06%	0.007%
83	12.542	3575	3577	3580	rVB4	1369	862	0.05%	0.007%
84	12.567	3583	3585	3586	rBV2	1528	572	0.04%	0.005%
85	12.712	3628	3630	3631	rBV2	1461	447	0.03%	0.004%
86	12.728	3632	3635	3637	rVV4	1405	740	0.05%	0.006%
87	12.799	3655	3657	3662	rVB5	1270	772	0.05%	0.006%
88	12.879	3680	3682	3684	rBV3	1139	532	0.03%	0.004%
89	13.014	3721	3724	3727	rBV3	1686	1445	0.09%	0.012%
90	13.075	3738	3743	3747	rBV8	2144	2021	0.13%	0.016%
91	13.355	3828	3830	3834	rVB5	1296	637	0.04%	0.005%
92	13.400	3842	3844	3847	rBV4	1747	1288	0.08%	0.010%
93	13.448	3851	3859	3869	rVV2	18474	31331	1.95%	0.251%
94	13.596	3898	3905	3906	rBV5	2125	2300	0.14%	0.018%
95	13.689	3923	3934	3947	rBV9	9927	19864	1.24%	0.159%
96	13.779	3960	3962	3965	rVB4	1856	968	0.06%	0.008%
97	13.799	3965	3968	3970	rBV4	1366	932	0.06%	0.007%
98	13.947	4012	4014	4015	rBV2	1027	450	0.03%	0.004%
99	14.062	4047	4050	4053	rBV5	1598	1065	0.07%	0.009%
100	14.242	4101	4106	4107	rBV5	2064	1491	0.09%	0.012%




Sum of corrected areas: 12494036

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032879.D
Acq On : 10 Nov 2023 10:03
Operator : SY/MD
Sample : VV1110WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

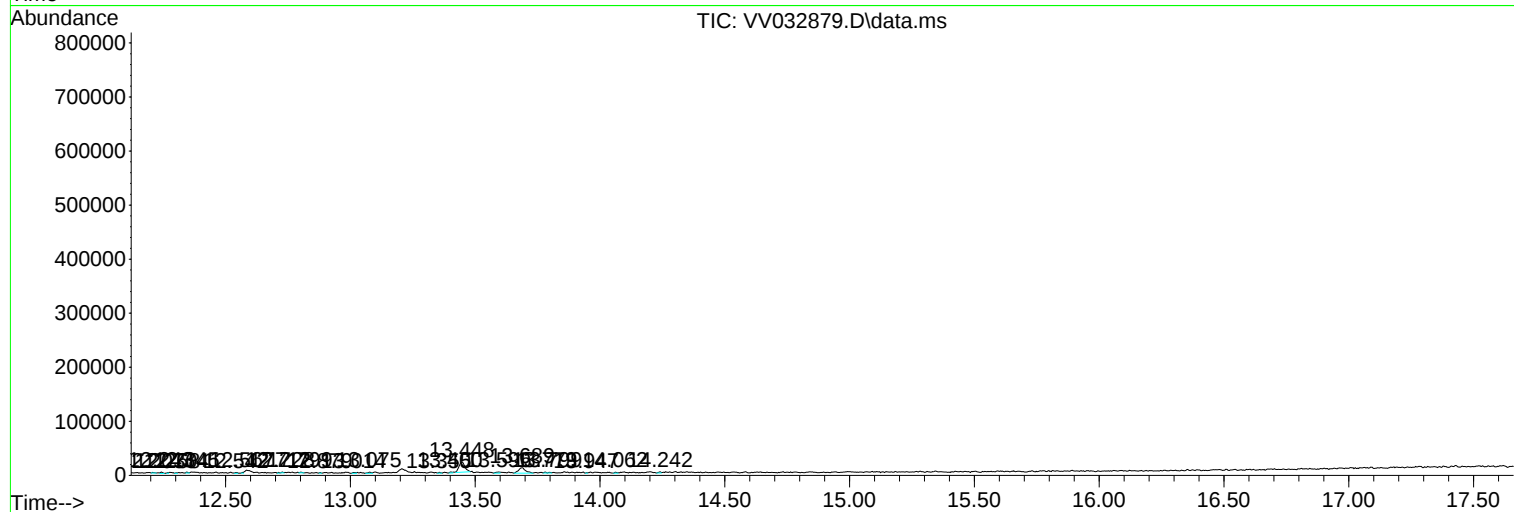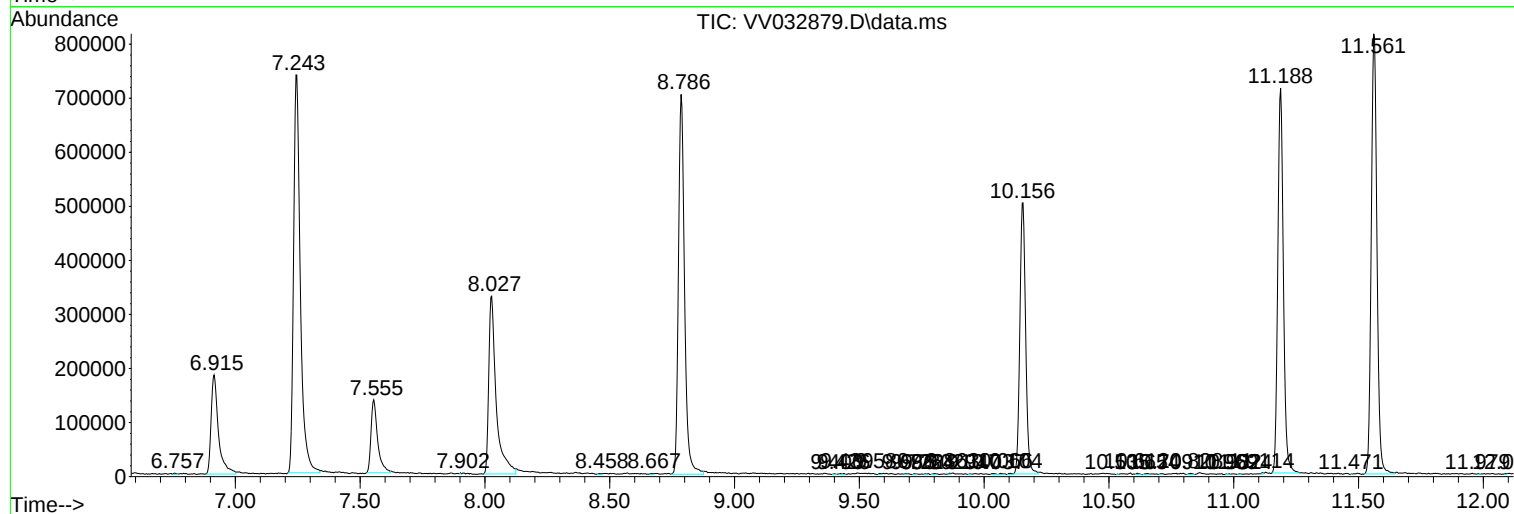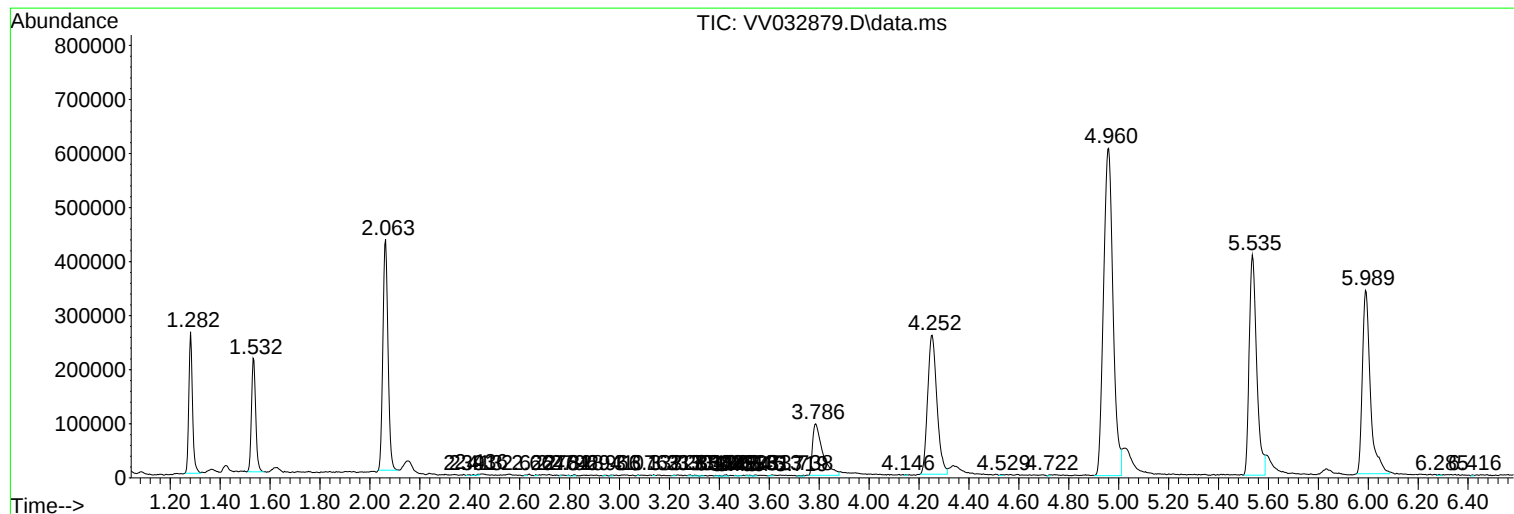

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032879.D
Acq On : 10 Nov 2023 10:03
Operator : SY/MD
Sample : VV1110WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032879.D
Acq On : 10 Nov 2023 10:03
Operator : SY/MD
Sample : VV1110WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK215

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------