

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032880.D
 Acq On : 10 Nov 2023 10:35
 Operator : SY/MD
 Sample : 05226-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032880.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.133	26	29	32	rBV4	2032	1487	0.09%	0.012%
2	1.281	68	75	90	rBV	250342	266168	15.42%	2.143%
3	1.532	147	153	165	rVB	205116	239027	13.85%	1.924%
4	2.059	309	317	330	rBV	415385	600255	34.77%	4.833%
5	2.375	412	415	418	rVB5	1674	1139	0.07%	0.009%
6	2.391	418	420	423	rBV4	1191	827	0.05%	0.007%
7	2.436	431	434	435	rBV2	2252	1172	0.07%	0.009%
8	2.539	461	466	468	rBV5	1417	1253	0.07%	0.010%
9	2.593	480	483	486	rBV5	764	686	0.04%	0.006%
10	2.635	494	496	498	rBV3	1314	706	0.04%	0.006%
11	2.735	526	527	529	rBV2	1283	680	0.04%	0.005%
12	2.773	537	539	542	rBV4	1494	789	0.05%	0.006%
13	2.799	544	547	548	rVV3	1274	587	0.03%	0.005%
14	2.883	569	573	575	rBV5	1440	924	0.05%	0.007%
15	2.895	575	577	580	rBV4	1787	1141	0.07%	0.009%
16	2.944	587	592	596	rBV7	1353	1655	0.10%	0.013%
17	3.031	616	619	620	rBV4	992	599	0.03%	0.005%
18	3.111	640	644	648	rVB7	1913	1528	0.09%	0.012%
19	3.133	648	651	654	rBV5	1047	757	0.04%	0.006%
20	3.188	665	668	673	rBV7	1387	1108	0.06%	0.009%
21	3.310	704	706	710	rVB4	976	640	0.04%	0.005%
22	3.362	717	722	726	rBV7	860	849	0.05%	0.007%
23	3.445	745	748	750	rBV4	1147	730	0.04%	0.006%
24	3.510	764	768	771	rBV5	1758	1297	0.08%	0.010%
25	3.555	780	782	784	rBV3	1612	906	0.05%	0.007%
26	3.641	805	809	814	rVB6	1894	1502	0.09%	0.012%
27	3.680	814	821	824	rBV7	1679	1720	0.10%	0.014%
28	3.786	845	854	876	rBV	79732	211111	12.23%	1.700%
29	4.104	951	953	960	rBV8	2180	1650	0.10%	0.013%
30	4.159	967	970	972	rBV4	1453	769	0.04%	0.006%
31	4.249	984	998	1019	rBV	256089	664651	38.50%	5.351%
32	4.805	1169	1171	1173	rBV3	1182	598	0.03%	0.005%
33	4.879	1192	1194	1197	rVB3	1991	1166	0.07%	0.009%
34	4.956	1200	1218	1263	rBV2	602504	1726359	100.00%	13.899%
35	5.448	1369	1371	1373	rBV3	1289	796	0.05%	0.006%
36	5.535	1386	1398	1435	rBV	407698	913225	52.90%	7.353%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032880.D
 Acq On : 10 Nov 2023 10:35
 Operator : SY/MD
 Sample : 05226-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	5.989	1526	1539	1567	rBV	341493	767708	44.47%	6.181%
38	6.288	1626	1632	1634	rBV6	1332	1457	0.08%	0.012%
39	6.362	1653	1655	1658	rBV4	1680	821	0.05%	0.007%
40	6.413	1667	1671	1673	rBV4	1759	1359	0.08%	0.011%
41	6.593	1725	1727	1729	rBV3	1181	607	0.04%	0.005%
42	6.763	1777	1780	1781	rVB3	1412	573	0.03%	0.005%
43	6.915	1817	1827	1849	rBV	179146	357470	20.71%	2.878%
44	7.243	1918	1929	1954	rBV	742043	1371970	79.47%	11.046%
45	7.554	2017	2026	2043	rBV	132684	242070	14.02%	1.949%
46	7.818	2106	2108	2109	rBV2	1582	693	0.04%	0.006%
47	7.969	2153	2155	2159	rBV4	1774	1450	0.08%	0.012%
48	8.027	2161	2173	2205	rBV	283373	603524	34.96%	4.859%
49	8.355	2273	2275	2276	rBV2	1861	891	0.05%	0.007%
50	8.625	2355	2359	2360	rBV4	1698	1137	0.07%	0.009%
51	8.715	2383	2387	2389	rBV4	1451	1030	0.06%	0.008%
52	8.734	2390	2393	2394	rBV3	1643	775	0.04%	0.006%
53	8.786	2398	2409	2431	rBV	691244	1175037	68.06%	9.460%
54	9.133	2514	2517	2519	rBV4	1828	1384	0.08%	0.011%
55	9.271	2558	2560	2562	rBV4	1087	693	0.04%	0.006%
56	9.400	2598	2600	2604	rBV5	1200	900	0.05%	0.007%
57	9.480	2621	2625	2627	rBV6	1545	1202	0.07%	0.010%
58	9.551	2643	2647	2648	rBV4	2218	1663	0.10%	0.013%
59	9.786	2718	2720	2724	rVB5	1710	1251	0.07%	0.010%
60	9.812	2724	2728	2731	rBV6	1596	1265	0.07%	0.010%
61	9.860	2740	2743	2744	rBV3	1751	776	0.04%	0.006%
62	9.889	2749	2752	2755	rBV5	1583	1025	0.06%	0.008%
63	10.037	2793	2798	2799	rBV4	1297	1204	0.07%	0.010%
64	10.152	2819	2834	2853	rBV	477437	774618	44.87%	6.237%
65	10.519	2944	2948	2950	rBV5	1645	1467	0.08%	0.012%
66	10.705	3003	3006	3007	rBV3	1438	764	0.04%	0.006%
67	10.844	3047	3049	3050	rBV2	1444	641	0.04%	0.005%
68	10.969	3085	3088	3091	rBV5	1693	1126	0.07%	0.009%
69	10.985	3091	3093	3095	rBV3	1279	682	0.04%	0.005%
70	11.188	3145	3156	3175	rBV	722550	1119017	64.82%	9.009%
71	11.451	3236	3238	3241	rBV3	1189	571	0.03%	0.005%
72	11.561	3261	3272	3293	rVV	806182	1286213	74.50%	10.356%
73	12.030	3414	3418	3421	rBV6	2077	1687	0.10%	0.014%
74	12.059	3425	3427	3432	rVV5	1207	925	0.05%	0.007%
75	12.117	3441	3445	3447	rBV5	1858	1450	0.08%	0.012%
76	12.149	3454	3455	3458	rBV3	1417	803	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032880.D
 Acq On : 10 Nov 2023 10:35
 Operator : SY/MD
 Sample : 05226-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	12.242	3480	3484	3485	rBV3	1527	824	0.05%	0.007%
78	12.307	3501	3504	3506	rBV4	1329	826	0.05%	0.007%
79	12.374	3521	3525	3530	rVB7	1780	1830	0.11%	0.015%
80	12.406	3530	3535	3537	rBV5	1712	1673	0.10%	0.013%
81	12.445	3545	3547	3548	rBV2	1125	577	0.03%	0.005%
82	12.541	3574	3577	3581	rBV5	1264	939	0.05%	0.008%
83	12.647	3608	3610	3611	rBV2	1806	801	0.05%	0.006%
84	12.738	3636	3638	3645	rVB8	1756	1618	0.09%	0.013%
85	12.779	3648	3651	3654	rVB4	1307	948	0.05%	0.008%
86	12.802	3654	3658	3660	rBV5	1981	1426	0.08%	0.011%
87	13.059	3735	3738	3740	rVV4	1430	845	0.05%	0.007%
88	13.133	3759	3761	3763	rBV3	1271	788	0.05%	0.006%
89	13.416	3847	3849	3851	rBV3	2277	870	0.05%	0.007%
90	13.445	3851	3858	3863	rBV2	11687	14972	0.87%	0.121%
91	13.538	3885	3887	3890	rBV3	1340	669	0.04%	0.005%
92	13.628	3910	3915	3917	rBV7	1889	1745	0.10%	0.014%
93	13.869	3985	3990	3995	rBV7	1843	1887	0.11%	0.015%
94	13.911	3998	4003	4004	rBV5	1275	762	0.04%	0.006%
95	14.043	4042	4044	4046	rVB3	1968	838	0.05%	0.007%
96	14.078	4050	4055	4056	rBV4	1934	1399	0.08%	0.011%
97	14.117	4066	4067	4071	rVB4	1703	783	0.05%	0.006%
98	14.194	4089	4091	4093	rBV3	1251	688	0.04%	0.006%
99	14.300	4120	4124	4127	rBV5	1466	1261	0.07%	0.010%
100	15.387	4460	4462	4464	rBV3	1684	1140	0.07%	0.009%


Sum of corrected areas: 12420465

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032880.D
Acq On : 10 Nov 2023 10:35
Operator : SY/MD
Sample : 05226-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

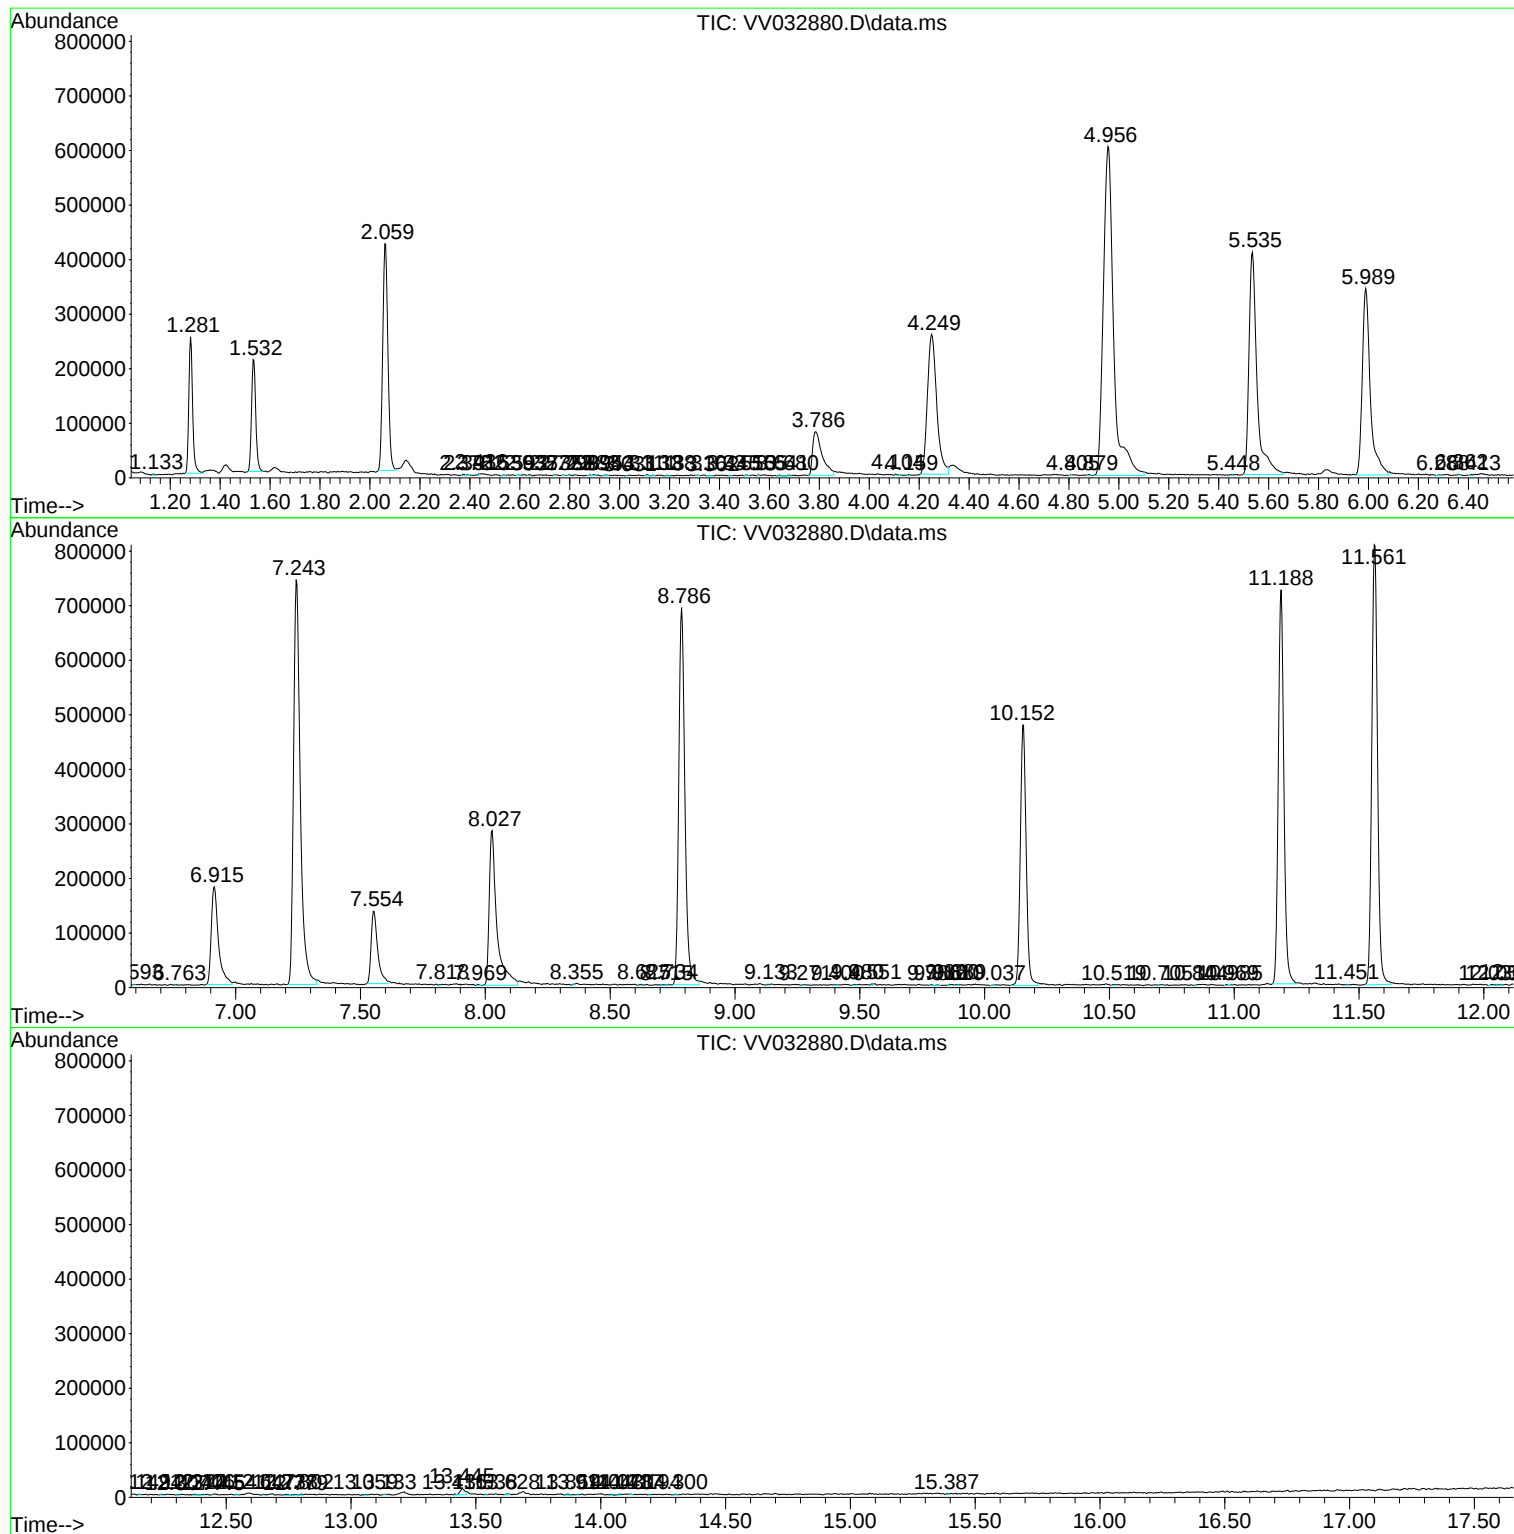

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032880.D
Acq On : 10 Nov 2023 10:35
Operator : SY/MD
Sample : 05226-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032880.D
Acq On : 10 Nov 2023 10:35
Operator : SY/MD
Sample : 05226-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc