

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032881.D
 Acq On : 10 Nov 2023 10:58
 Operator : SY/MD
 Sample : 05259-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032881.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	88	rBV	247390	255354	15.99%	2.096%
2	1.535	147	154	169	rVB	210503	245543	15.38%	2.016%
3	2.063	309	318	334	rBV	422553	608287	38.10%	4.993%
4	2.535	461	465	467	rVV5	1349	974	0.06%	0.008%
5	2.709	516	519	522	rVB5	1726	1185	0.07%	0.010%
6	2.725	522	524	525	rBV2	1287	577	0.04%	0.005%
7	2.767	533	537	539	rBV5	1818	1429	0.09%	0.012%
8	2.822	552	554	556	rBV3	1866	731	0.05%	0.006%
9	2.850	560	563	566	rBV4	1365	1016	0.06%	0.008%
10	2.886	571	574	575	rBV2	1539	957	0.06%	0.008%
11	2.992	605	607	609	rBV3	992	513	0.03%	0.004%
12	3.050	622	625	628	rVV5	1095	739	0.05%	0.006%
13	3.117	644	646	650	rVB4	1376	804	0.05%	0.007%
14	3.162	658	660	662	rBV3	1197	763	0.05%	0.006%
15	3.275	694	695	697	rBV2	1167	517	0.03%	0.004%
16	3.384	724	729	732	rVB6	1545	1484	0.09%	0.012%
17	3.461	748	753	754	rBV4	1591	1070	0.07%	0.009%
18	3.516	768	770	772	rBV2	1199	606	0.04%	0.005%
19	3.593	791	794	795	rBV3	1245	637	0.04%	0.005%
20	3.789	846	855	884	rBV	89771	253053	15.85%	2.077%
21	4.104	951	953	955	rVB3	2307	999	0.06%	0.008%
22	4.252	984	999	1020	rBV	256258	671227	42.04%	5.510%
23	4.587	1100	1103	1106	rBV5	1730	1214	0.08%	0.010%
24	4.638	1116	1119	1121	rBV4	2001	1052	0.07%	0.009%
25	4.735	1143	1149	1153	rBV8	1922	1970	0.12%	0.016%
26	4.802	1167	1170	1179	rVB8	1619	2035	0.13%	0.017%
27	4.838	1179	1181	1183	rBV3	1057	617	0.04%	0.005%
28	4.883	1193	1195	1196	rBV2	1308	649	0.04%	0.005%
29	4.960	1203	1219	1235	rBV3	607387	1596553	100.00%	13.106%
30	5.333	1332	1335	1337	rBV4	2149	1050	0.07%	0.009%
31	5.429	1360	1365	1367	rBV6	2038	1588	0.10%	0.013%
32	5.538	1387	1399	1434	rBV	367634	834060	52.24%	6.847%
33	5.992	1528	1540	1570	rBV2	337402	756795	47.40%	6.212%
34	6.352	1649	1652	1653	rBV3	1336	579	0.04%	0.005%
35	6.635	1737	1740	1741	rBV3	1810	857	0.05%	0.007%
36	6.796	1786	1790	1793	rBV6	1378	852	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032881.D
 Acq On : 10 Nov 2023 10:58
 Operator : SY/MD
 Sample : 05259-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	6.915	1817	1827	1851	rBV	180513	361758	22.66%	2.970%
38	7.111	1886	1888	1890	rBV2	1503	601	0.04%	0.005%
39	7.246	1918	1930	1965	rBV	734422	1385446	86.78%	11.373%
40	7.554	2017	2026	2050	rBV	134298	254669	15.95%	2.091%
41	7.699	2068	2071	2073	rBV4	2231	1565	0.10%	0.013%
42	8.027	2163	2173	2204	rBV	322710	665994	41.71%	5.467%
43	8.542	2331	2333	2336	rBV3	1513	1020	0.06%	0.008%
44	8.657	2365	2369	2372	rBV5	1971	1975	0.12%	0.016%
45	8.712	2383	2386	2388	rBV4	1847	1365	0.09%	0.011%
46	8.786	2398	2409	2434	rBV	639753	1077746	67.50%	8.847%
47	9.117	2510	2512	2519	rVB8	2636	1991	0.12%	0.016%
48	9.220	2542	2544	2547	rBV4	1500	1050	0.07%	0.009%
49	9.287	2562	2565	2568	rBV5	1494	1099	0.07%	0.009%
50	9.381	2592	2594	2596	rBV3	1218	718	0.04%	0.006%
51	9.403	2598	2601	2603	rBV4	2396	1438	0.09%	0.012%
52	9.458	2616	2618	2623	rVB5	1968	1208	0.08%	0.010%
53	9.490	2623	2628	2630	rBV6	1714	1637	0.10%	0.013%
54	9.525	2637	2639	2644	rBV7	1999	1486	0.09%	0.012%
55	9.818	2724	2730	2734	rBV7	2189	2261	0.14%	0.019%
56	9.882	2746	2750	2757	rVB9	1813	2368	0.15%	0.019%
57	9.927	2761	2764	2766	rBV3	1493	961	0.06%	0.008%
58	9.988	2781	2783	2784	rBV2	1367	614	0.04%	0.005%
59	10.040	2796	2799	2801	rBV4	1461	942	0.06%	0.008%
60	10.114	2820	2822	2823	rBV2	2312	1084	0.07%	0.009%
61	10.156	2824	2835	2851	rVV	499104	799599	50.08%	6.564%
62	10.609	2974	2976	2977	rBV2	1343	599	0.04%	0.005%
63	10.660	2987	2992	2994	rVB6	2128	1616	0.10%	0.013%
64	10.686	2996	3000	3002	rBV4	1710	1363	0.09%	0.011%
65	10.869	3055	3057	3060	rBV4	2455	1475	0.09%	0.012%
66	10.998	3094	3097	3099	rBV4	1160	588	0.04%	0.005%
67	11.024	3103	3105	3108	rBV4	1418	871	0.05%	0.007%
68	11.188	3145	3156	3178	rBV	650652	1023049	64.08%	8.398%
69	11.445	3234	3236	3240	rVB5	1347	772	0.05%	0.006%
70	11.522	3256	3260	3261	rBV3	1165	949	0.06%	0.008%
71	11.564	3261	3273	3291	rVV	806061	1283619	80.40%	10.537%
72	11.840	3353	3359	3362	rBV8	1803	1812	0.11%	0.015%
73	12.011	3411	3412	3416	rVB4	1233	678	0.04%	0.006%
74	12.123	3445	3447	3450	rBV4	1352	768	0.05%	0.006%
75	12.525	3570	3572	3574	rBV3	1679	842	0.05%	0.007%
76	12.590	3586	3592	3598	rBV3	3585	5387	0.34%	0.044%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032881.D
 Acq On : 10 Nov 2023 10:58
 Operator : SY/MD
 Sample : 05259-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	12.683	3619	3621	3624	rVB4	1406	805	0.05%	0.007%
78	12.776	3646	3650	3653	rBV5	1691	1457	0.09%	0.012%
79	12.837	3666	3669	3672	rBV5	1201	798	0.05%	0.007%
80	12.947	3700	3703	3704	rBV3	1554	642	0.04%	0.005%
81	12.979	3711	3713	3715	rVB2	2192	845	0.05%	0.007%
82	13.030	3723	3729	3730	rBV6	1857	1800	0.11%	0.015%
83	13.062	3737	3739	3744	rVB5	2181	1535	0.10%	0.013%
84	13.094	3744	3749	3753	rBV8	1982	2248	0.14%	0.018%
85	13.204	3775	3783	3784	rBV6	3982	4799	0.30%	0.039%
86	13.271	3800	3804	3806	rBV5	1346	1131	0.07%	0.009%
87	13.374	3833	3836	3837	rBV3	1022	570	0.04%	0.005%
88	13.384	3837	3839	3844	rVB6	1593	1086	0.07%	0.009%
89	13.451	3851	3860	3869	rBV5	6378	11388	0.71%	0.093%
90	13.580	3897	3900	3901	rBV3	1072	500	0.03%	0.004%
91	13.757	3951	3955	3957	rVB4	1703	1165	0.07%	0.010%
92	13.770	3957	3959	3961	rBV3	1422	843	0.05%	0.007%
93	14.046	4039	4045	4050	rVB10	1377	1324	0.08%	0.011%
94	14.098	4060	4061	4062	rBV	1513	511	0.03%	0.004%
95	14.117	4065	4067	4069	rVB3	1575	616	0.04%	0.005%
96	14.200	4090	4093	4094	rBV3	1255	663	0.04%	0.005%
97	14.355	4139	4141	4143	rBV2	1250	782	0.05%	0.006%
98	14.480	4178	4180	4184	rBV4	1331	1065	0.07%	0.009%
99	14.567	4205	4207	4208	rBV2	1603	577	0.04%	0.005%
100	15.184	4397	4399	4401	rBV2	2818	1721	0.11%	0.014%




Sum of corrected areas: 12182190

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032881.D
Acq On : 10 Nov 2023 10:58
Operator : SY/MD
Sample : 05259-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

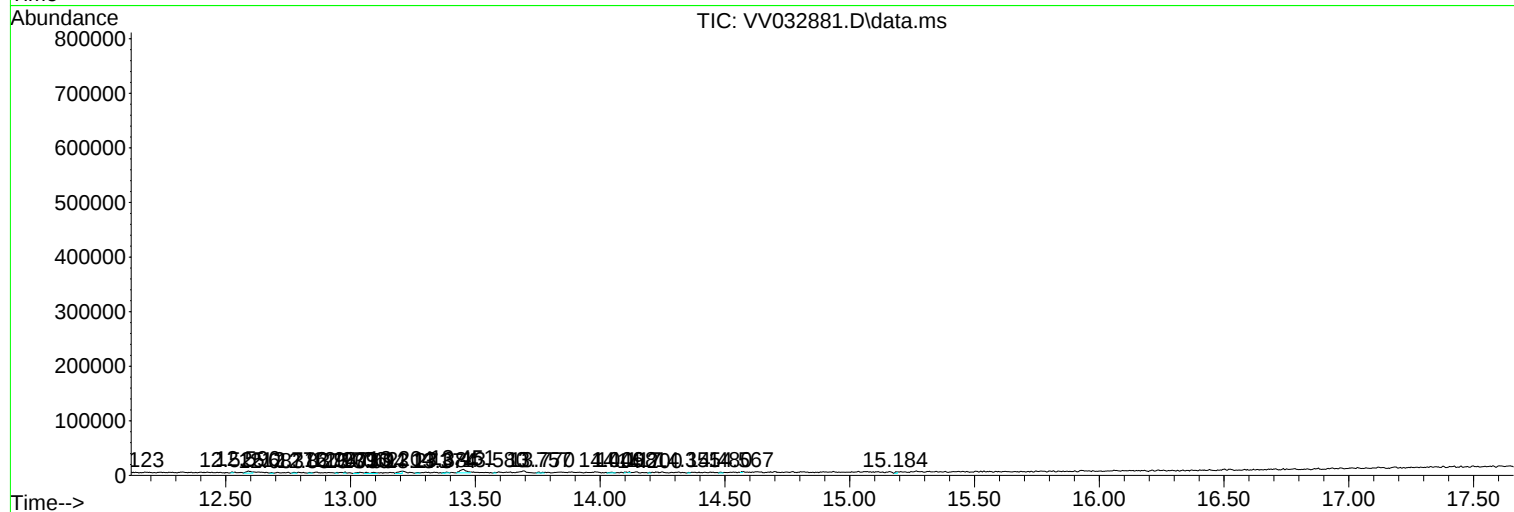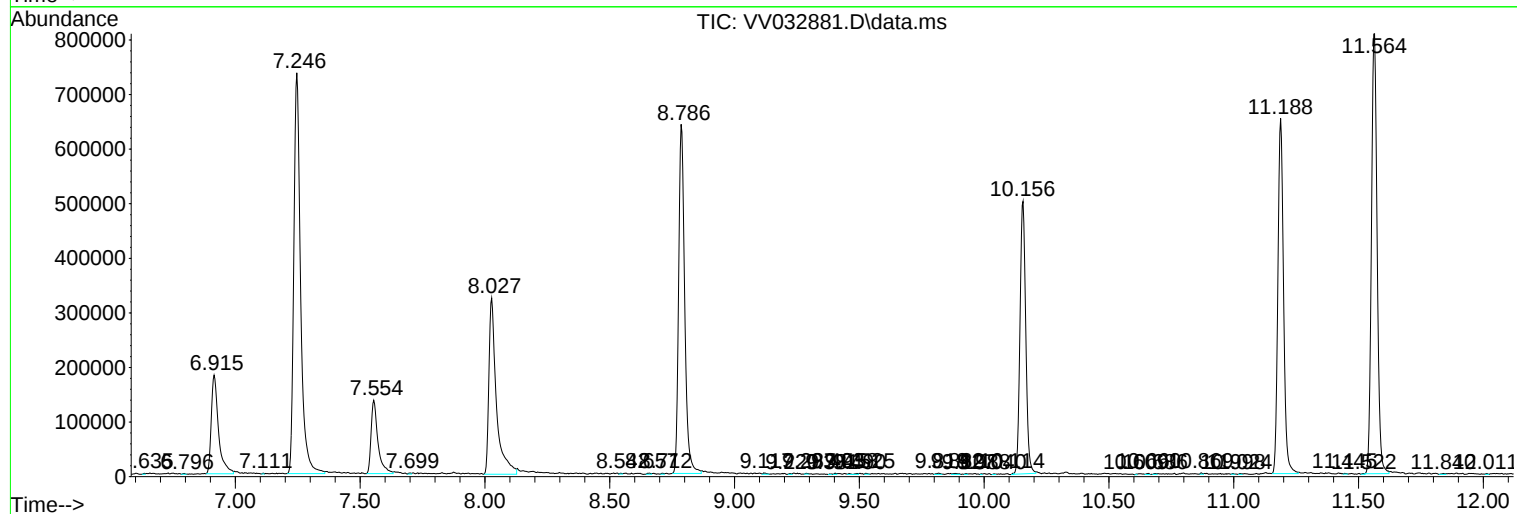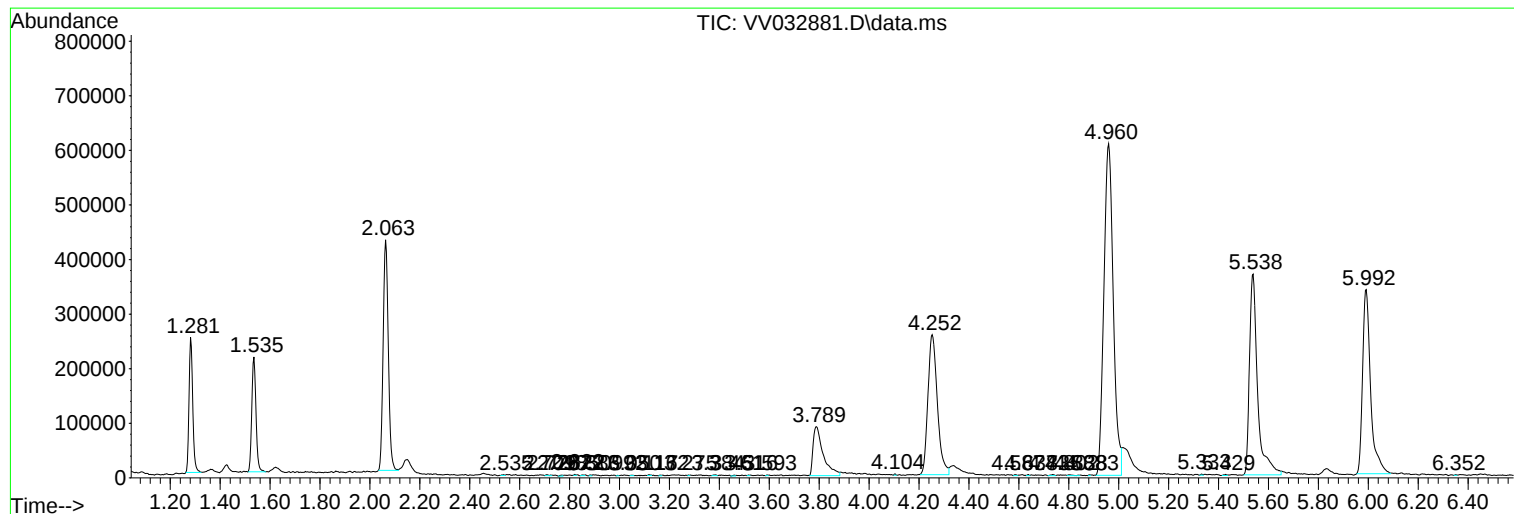

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032881.D
Acq On : 10 Nov 2023 10:58
Operator : SY/MD
Sample : 05259-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032881.D
Acq On : 10 Nov 2023 10:58
Operator : SY/MD
Sample : 05259-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------