

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032883.D
 Acq On : 10 Nov 2023 11:47
 Operator : SY/MD
 Sample : 05333-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032883.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	89	rBV	180883	189389	15.81%	1.950%
2	1.532	146	153	168	rVB	160740	190206	15.87%	1.958%
3	2.060	309	317	329	rBV	307523	443490	37.01%	4.566%
4	2.327	396	400	402	rBV5	2530	1488	0.12%	0.015%
5	2.529	461	463	467	rBV4	1263	818	0.07%	0.008%
6	2.892	572	576	577	rBV4	1295	647	0.05%	0.007%
7	2.941	589	591	594	rVB4	1243	671	0.06%	0.007%
8	2.957	594	596	598	rBV3	1104	758	0.06%	0.008%
9	2.973	598	601	605	rVB6	1305	1076	0.09%	0.011%
10	3.008	609	612	614	rBV3	1569	1197	0.10%	0.012%
11	3.044	621	623	627	rBV5	934	683	0.06%	0.007%
12	3.137	649	652	653	rBV3	1731	869	0.07%	0.009%
13	3.224	677	679	683	rVV5	1139	952	0.08%	0.010%
14	3.281	695	697	699	rBV3	1079	664	0.06%	0.007%
15	3.378	724	727	728	rBV3	2183	909	0.08%	0.009%
16	3.397	731	733	738	rVB6	1538	1093	0.09%	0.011%
17	3.426	738	742	744	rBV5	1836	1176	0.10%	0.012%
18	3.442	744	747	749	rVB4	1452	771	0.06%	0.008%
19	3.513	766	769	771	rBV5	1516	953	0.08%	0.010%
20	3.558	780	783	786	rBV5	1473	893	0.07%	0.009%
21	3.600	793	796	799	rBV6	1282	828	0.07%	0.009%
22	3.683	819	822	824	rBV4	1744	1368	0.11%	0.014%
23	3.738	837	839	842	rBV4	1098	876	0.07%	0.009%
24	3.789	846	855	885	rVV	69828	195549	16.32%	2.013%
25	4.252	985	999	1019	rBV	194453	509398	42.51%	5.244%
26	4.468	1062	1066	1067	rBV4	2526	1667	0.14%	0.017%
27	4.593	1103	1105	1109	rBV5	1477	703	0.06%	0.007%
28	4.613	1109	1111	1117	rVB5	2714	2080	0.17%	0.021%
29	4.645	1117	1121	1124	rBV6	1863	1656	0.14%	0.017%
30	4.703	1137	1139	1140	rBV2	1530	668	0.06%	0.007%
31	4.780	1160	1163	1165	rBV3	948	726	0.06%	0.007%
32	4.960	1203	1219	1236	rBV2	451850	1198251	100.00%	12.336%
33	5.285	1313	1320	1322	rBV5	2388	2260	0.19%	0.023%
34	5.381	1348	1350	1352	rBV3	1203	686	0.06%	0.007%
35	5.535	1385	1398	1414	rBV	358160	749776	62.57%	7.719%
36	5.989	1524	1539	1572	rBV	260919	600631	50.13%	6.184%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032883.D
 Acq On : 10 Nov 2023 11:47
 Operator : SY/MD
 Sample : 05333-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	6.915	1818	1827	1859	rVB	133474	270809	22.60%	2.788%
38	7.127	1889	1893	1897	rBV6	1382	1382	0.12%	0.014%
39	7.246	1918	1930	1954	rBV	535669	1008584	84.17%	10.383%
40	7.519	2013	2015	2016	rBV2	1683	700	0.06%	0.007%
41	7.555	2018	2026	2047	rVV	98081	185304	15.46%	1.908%
42	7.960	2148	2152	2154	rBV5	1130	874	0.07%	0.009%
43	7.973	2154	2156	2160	rBV5	1454	959	0.08%	0.010%
44	8.027	2164	2173	2205	rBV	236391	513658	42.87%	5.288%
45	8.436	2298	2300	2302	rBV3	1793	1151	0.10%	0.012%
46	8.481	2311	2314	2317	rBV5	1805	1559	0.13%	0.016%
47	8.542	2330	2333	2337	rBV6	1900	1534	0.13%	0.016%
48	8.619	2354	2357	2358	rBV3	1562	907	0.08%	0.009%
49	8.715	2386	2387	2391	rVB4	1332	721	0.06%	0.007%
50	8.744	2393	2396	2398	rBV3	1381	686	0.06%	0.007%
51	8.786	2398	2409	2437	rBV	607273	1040763	86.86%	10.715%
52	9.230	2544	2547	2550	rBV6	1003	883	0.07%	0.009%
53	9.255	2551	2555	2558	rVV6	1797	1539	0.13%	0.016%
54	9.284	2562	2564	2568	rVB4	1533	991	0.08%	0.010%
55	9.352	2582	2585	2589	rBV6	1574	1152	0.10%	0.012%
56	9.381	2592	2594	2597	rBV3	1492	934	0.08%	0.010%
57	9.426	2606	2608	2612	rVB6	1584	987	0.08%	0.010%
58	9.448	2612	2615	2618	rVB4	2653	1432	0.12%	0.015%
59	9.468	2618	2621	2623	rBV4	1480	774	0.06%	0.008%
60	9.545	2642	2645	2649	rBV6	1772	1182	0.10%	0.012%
61	9.677	2683	2686	2690	rBV6	1354	1119	0.09%	0.012%
62	9.809	2725	2727	2730	rBV3	982	768	0.06%	0.008%
63	9.937	2765	2767	2772	rBV6	1329	1206	0.10%	0.012%
64	9.992	2782	2784	2788	rBV5	1336	905	0.08%	0.009%
65	10.024	2788	2794	2796	rBV6	1619	1626	0.14%	0.017%
66	10.091	2812	2815	2818	rBV4	1692	1017	0.08%	0.010%
67	10.108	2818	2820	2822	rVV3	1329	733	0.06%	0.008%
68	10.156	2824	2835	2857	rVV	389273	621857	51.90%	6.402%
69	10.355	2895	2897	2899	rBV3	2192	1221	0.10%	0.013%
70	10.461	2928	2930	2934	rVB4	1787	1078	0.09%	0.011%
71	10.484	2934	2937	2941	rBV5	1570	1566	0.13%	0.016%
72	10.571	2961	2964	2968	rBV6	1375	935	0.08%	0.010%
73	10.654	2987	2990	2993	rBV5	1234	977	0.08%	0.010%
74	10.866	3052	3056	3058	rBV4	2393	1848	0.15%	0.019%
75	10.879	3058	3060	3065	rVB5	1781	1099	0.09%	0.011%
76	10.911	3065	3070	3071	rBV3	1450	1088	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032883.D
 Acq On : 10 Nov 2023 11:47
 Operator : SY/MD
 Sample : 05333-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCGD5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	11.040	3108	3110	3112	rBV3	1554	796	0.07%	0.008%
78	11.188	3145	3156	3178	rBV	602218	943704	78.76%	9.715%
79	11.564	3260	3273	3292	rBV	611991	958044	79.95%	9.863%
80	11.773	3335	3338	3342	rBV5	2370	2039	0.17%	0.021%
81	12.034	3417	3419	3422	rBV4	1690	831	0.07%	0.009%
82	12.124	3443	3447	3450	rBV6	1996	1796	0.15%	0.018%
83	12.198	3466	3470	3471	rBV3	1473	1044	0.09%	0.011%
84	12.239	3481	3483	3487	rVB5	2209	1494	0.12%	0.015%
85	12.493	3560	3562	3565	rBV4	1226	582	0.05%	0.006%
86	12.644	3606	3609	3610	rBV2	1468	704	0.06%	0.007%
87	12.715	3629	3631	3635	rVB5	1122	690	0.06%	0.007%
88	12.734	3635	3637	3639	rBV3	1509	825	0.07%	0.008%
89	12.789	3651	3654	3657	rVB5	1559	850	0.07%	0.009%
90	12.805	3657	3659	3662	rVV4	1664	756	0.06%	0.008%
91	12.943	3699	3702	3704	rBV4	1760	1098	0.09%	0.011%
92	13.349	3825	3828	3829	rBV3	1653	985	0.08%	0.010%
93	13.455	3855	3861	3864	rBV5	4019	5123	0.43%	0.053%
94	13.574	3895	3898	3899	rBV2	1820	1120	0.09%	0.012%
95	13.754	3952	3954	3956	rBV3	1481	668	0.06%	0.007%
96	13.815	3971	3973	3978	rVB6	1359	974	0.08%	0.010%
97	14.088	4054	4058	4060	rBV4	1698	1302	0.11%	0.013%
98	14.101	4060	4062	4064	rBV3	1359	614	0.05%	0.006%
99	14.310	4124	4127	4131	rBV5	1884	1566	0.13%	0.016%
100	14.535	4195	4197	4200	rBV3	2067	1508	0.13%	0.016%

Sum of corrected areas: 9713447




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032883.D
Acq On : 10 Nov 2023 11:47
Operator : SY/MD
Sample : 05333-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

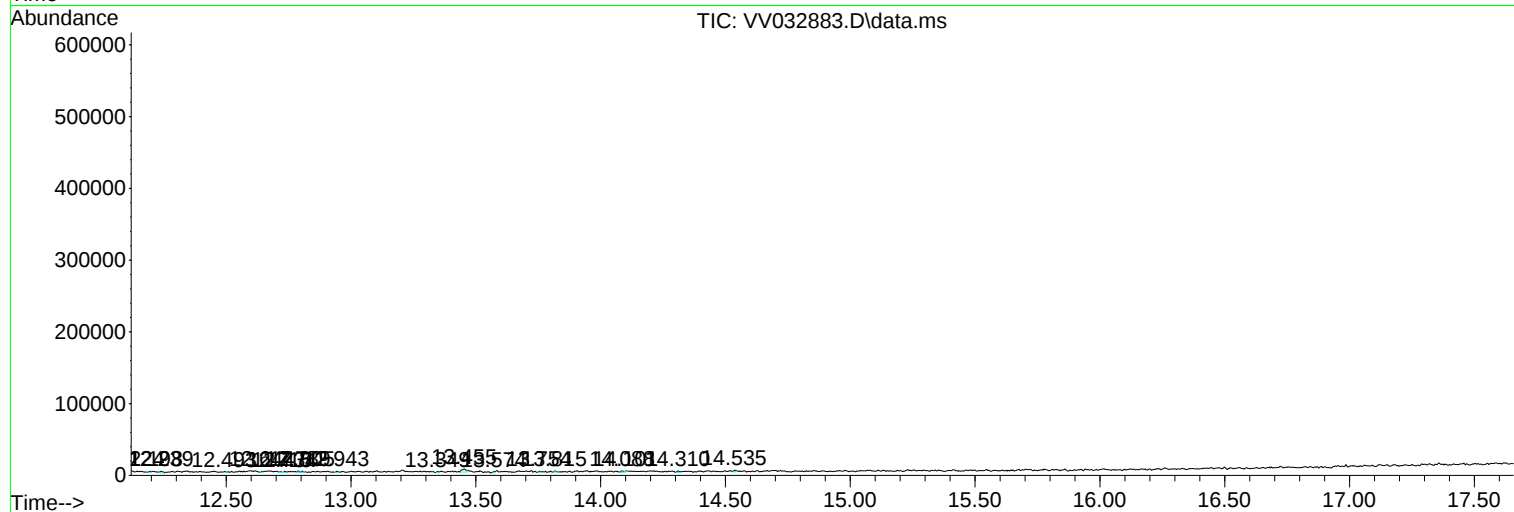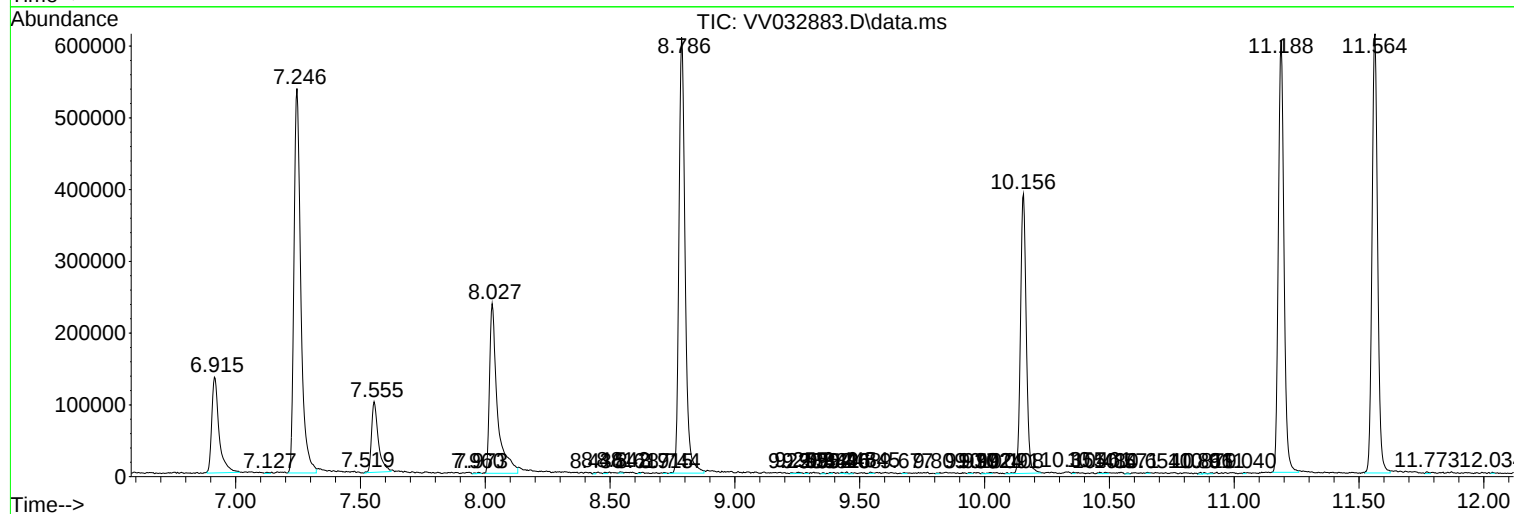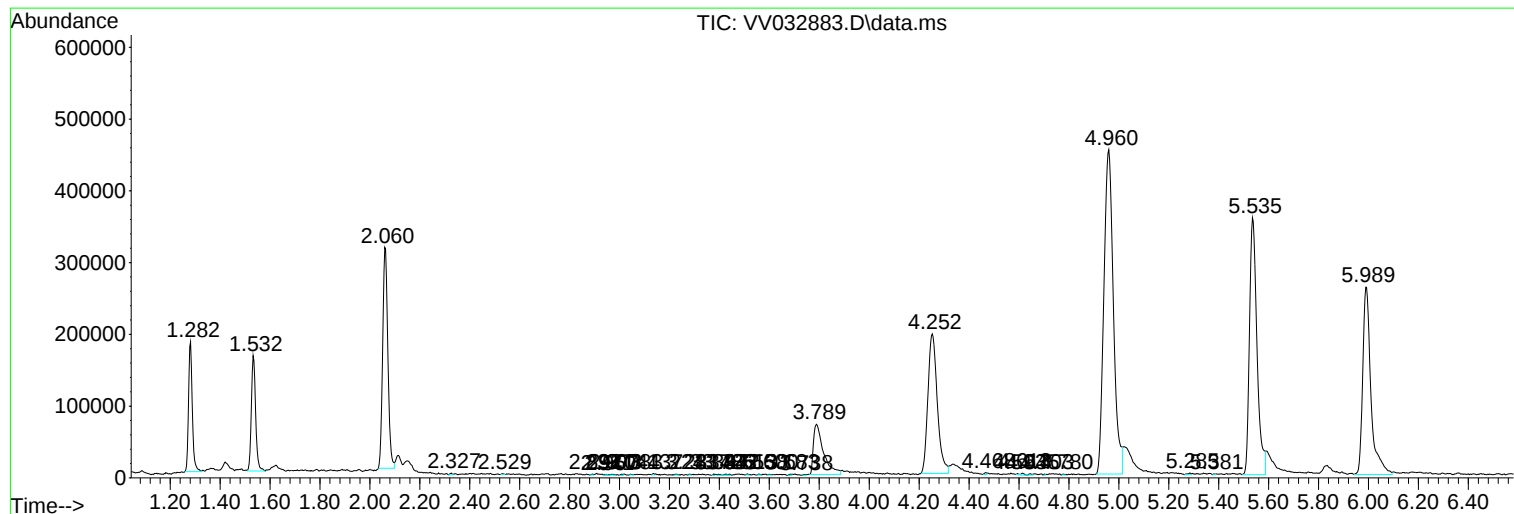

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032883.D
Acq On : 10 Nov 2023 11:47
Operator : SY/MD
Sample : 05333-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032883.D
Acq On : 10 Nov 2023 11:47
Operator : SY/MD
Sample : 05333-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCGD5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------