

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032884.D
 Acq On : 10 Nov 2023 12:11
 Operator : SY/MD
 Sample : 05326-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E45K1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032884.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	91	rVB	211777	220394	15.02%	1.761%
2	1.535	147	154	166	rVB	190652	218889	14.92%	1.749%
3	2.063	309	318	330	rBV	371592	532961	36.33%	4.257%
4	2.432	429	433	434	rBV3	1577	1235	0.08%	0.010%
5	2.680	508	510	511	rBV3	1372	675	0.05%	0.005%
6	2.767	536	537	539	rVB2	1129	245	0.02%	0.002%
7	2.857	564	565	566	rBV	1018	298	0.02%	0.002%
8	2.944	589	592	594	rVB4	1401	747	0.05%	0.006%
9	3.021	614	616	620	rBV5	862	481	0.03%	0.004%
10	3.082	633	635	638	rBV4	1182	538	0.04%	0.004%
11	3.162	658	660	664	rVB4	1678	957	0.07%	0.008%
12	3.182	664	666	668	rBV3	1179	574	0.04%	0.005%
13	3.259	688	690	693	rBV3	1614	1295	0.09%	0.010%
14	3.313	704	707	710	rVB4	1404	885	0.06%	0.007%
15	3.368	721	724	725	rBV3	1082	570	0.04%	0.005%
16	3.391	725	731	741	rVV3	1879	3496	0.24%	0.028%
17	3.474	754	757	759	rBV3	1364	1075	0.07%	0.009%
18	3.529	772	774	776	rBV3	1219	681	0.05%	0.005%
19	3.561	782	784	785	rBV	671	166	0.01%	0.001%
20	3.658	812	814	815	rBV2	1701	575	0.04%	0.005%
21	3.696	824	826	828	rBV3	1281	481	0.03%	0.004%
22	3.786	846	854	881	rBV	83617	232484	15.85%	1.857%
23	4.252	985	999	1019	rBV	236373	607788	41.43%	4.855%
24	4.558	1092	1094	1096	rBV3	1585	653	0.04%	0.005%
25	4.696	1136	1137	1139	rVB2	939	292	0.02%	0.002%
26	4.841	1180	1182	1183	rBV2	1039	259	0.02%	0.002%
27	4.892	1196	1198	1199	rBV2	1068	296	0.02%	0.002%
28	4.960	1203	1219	1236	rBV2	545148	1466917	100.00%	11.718%
29	5.535	1388	1398	1441	rVB	390024	866298	59.06%	6.920%
30	5.841	1483	1493	1517	rVB9	22472	62421	4.26%	0.499%
31	5.992	1528	1540	1573	rBV	319622	705952	48.12%	5.639%
32	6.468	1686	1688	1691	rVB3	1353	416	0.03%	0.003%
33	6.706	1760	1762	1764	rBV4	1110	710	0.05%	0.006%
34	6.818	1794	1797	1798	rBV3	1276	601	0.04%	0.005%
35	6.915	1818	1827	1853	rBV	161601	322559	21.99%	2.577%
36	7.246	1919	1930	1961	rBV	666201	1231842	83.97%	9.840%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032884.D
 Acq On : 10 Nov 2023 12:11
 Operator : SY/MD
 Sample : 05326-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E45K1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	7.554	2017	2026	2046	rBV	120659	226678	15.45%	1.811%
38	7.751	2083	2087	2088	rBV3	1582	1266	0.09%	0.010%
39	7.908	2124	2136	2163	rVB	565683	1007894	68.71%	8.051%
40	8.027	2164	2173	2206	rBV	298567	608217	41.46%	4.859%
41	8.786	2398	2409	2436	rBV	690962	1167795	79.61%	9.329%
42	9.339	2580	2581	2585	rVB4	2081	1110	0.08%	0.009%
43	9.365	2585	2589	2590	rBV4	1097	750	0.05%	0.006%
44	9.432	2608	2610	2611	rBV2	937	367	0.03%	0.003%
45	9.442	2611	2613	2618	rVV6	1802	1190	0.08%	0.010%
46	9.535	2639	2642	2643	rBV3	1006	554	0.04%	0.004%
47	9.757	2709	2711	2714	rBV4	2156	1219	0.08%	0.010%
48	9.770	2714	2715	2720	rVB5	1809	1261	0.09%	0.010%
49	9.812	2726	2728	2734	rVB6	2346	1627	0.11%	0.013%
50	9.879	2746	2749	2754	rVB6	2415	2012	0.14%	0.016%
51	9.905	2754	2757	2759	rBV4	1645	1077	0.07%	0.009%
52	9.982	2779	2781	2784	rBV3	1416	948	0.06%	0.008%
53	10.156	2823	2835	2857	rBV	479732	758843	51.73%	6.062%
54	10.574	2962	2965	2966	rBV2	1185	473	0.03%	0.004%
55	10.586	2966	2969	2971	rVV4	1329	784	0.05%	0.006%
56	10.718	3008	3010	3011	rBV2	1427	555	0.04%	0.004%
57	10.914	3069	3071	3072	rBV2	1081	532	0.04%	0.004%
58	10.937	3075	3078	3079	rVV2	1250	530	0.04%	0.004%
59	11.014	3100	3102	3103	rBV2	1025	352	0.02%	0.003%
60	11.188	3144	3156	3172	rBV	683278	1051555	71.68%	8.400%
61	11.564	3261	3273	3290	rBV	746479	1171089	79.83%	9.355%
62	11.882	3370	3372	3376	rVB5	2512	1514	0.10%	0.012%
63	11.950	3389	3393	3395	rBV5	2629	2222	0.15%	0.018%
64	12.008	3409	3411	3413	rBV3	1571	1074	0.07%	0.009%
65	12.056	3424	3426	3427	rBV3	1285	483	0.03%	0.004%
66	12.133	3446	3450	3452	rBV4	2102	1655	0.11%	0.013%
67	12.194	3465	3469	3470	rBV4	2161	1171	0.08%	0.009%
68	12.413	3535	3537	3538	rBV2	1322	432	0.03%	0.003%
69	12.464	3551	3553	3555	rBV3	1378	812	0.06%	0.006%
70	12.493	3560	3562	3564	rBV3	1156	533	0.04%	0.004%
71	12.564	3581	3584	3586	rBV4	1411	984	0.07%	0.008%
72	12.580	3586	3589	3591	rBV3	2208	1647	0.11%	0.013%
73	12.799	3654	3657	3658	rBV3	1314	741	0.05%	0.006%
74	12.966	3706	3709	3711	rBV3	1098	751	0.05%	0.006%
75	13.027	3726	3728	3731	rVB2	1122	663	0.05%	0.005%
76	13.043	3731	3733	3736	rBV4	1639	940	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032884.D
Acq On : 10 Nov 2023 12:11
Operator : SY/MD
Sample : 05326-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E45K1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M

Title : VOC Analysis

77	13.249	3795	3797	3798	rBV2	1129	535	0.04%	0.004%
78	13.319	3815	3819	3822	rBV6	2644	2203	0.15%	0.018%
79	13.403	3843	3845	3847	rBV2	1496	837	0.06%	0.007%
80	13.426	3850	3852	3853	rBV2	1769	849	0.06%	0.007%
81	13.869	3987	3990	3993	rBV5	1866	1403	0.10%	0.011%
82	14.043	4042	4044	4047	rVB4	1879	993	0.07%	0.008%
83	14.120	4066	4068	4070	rBV3	1465	546	0.04%	0.004%




Sum of corrected areas: 12518372

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032884.D
Acq On : 10 Nov 2023 12:11
Operator : SY/MD
Sample : 05326-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E45K1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

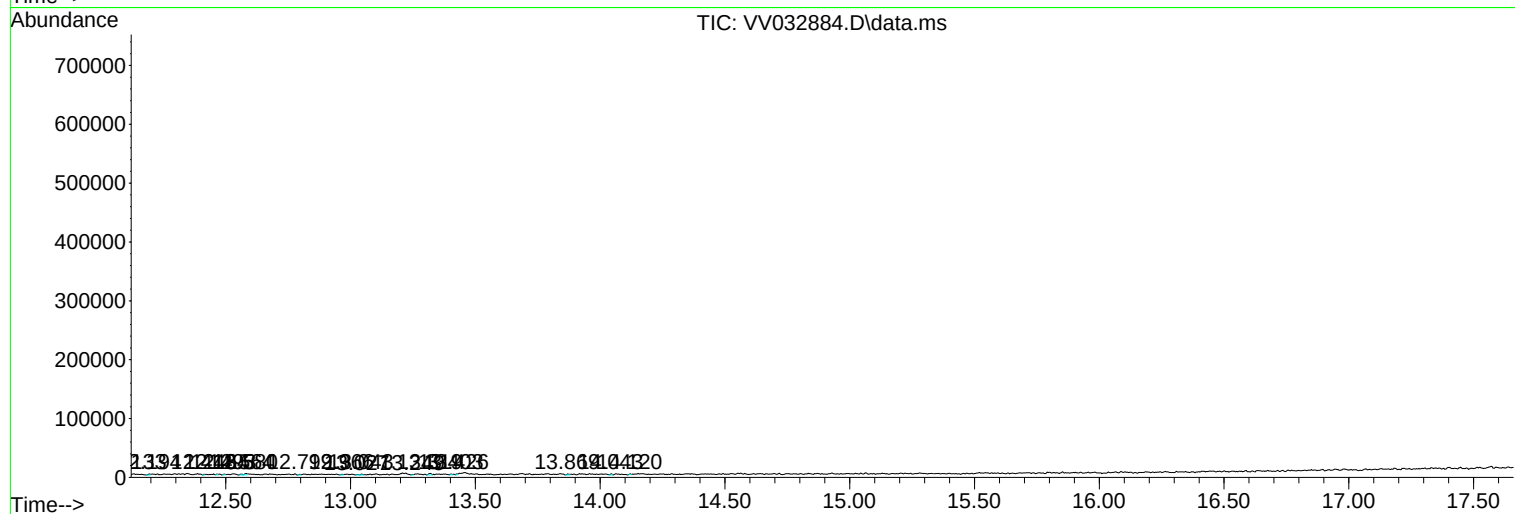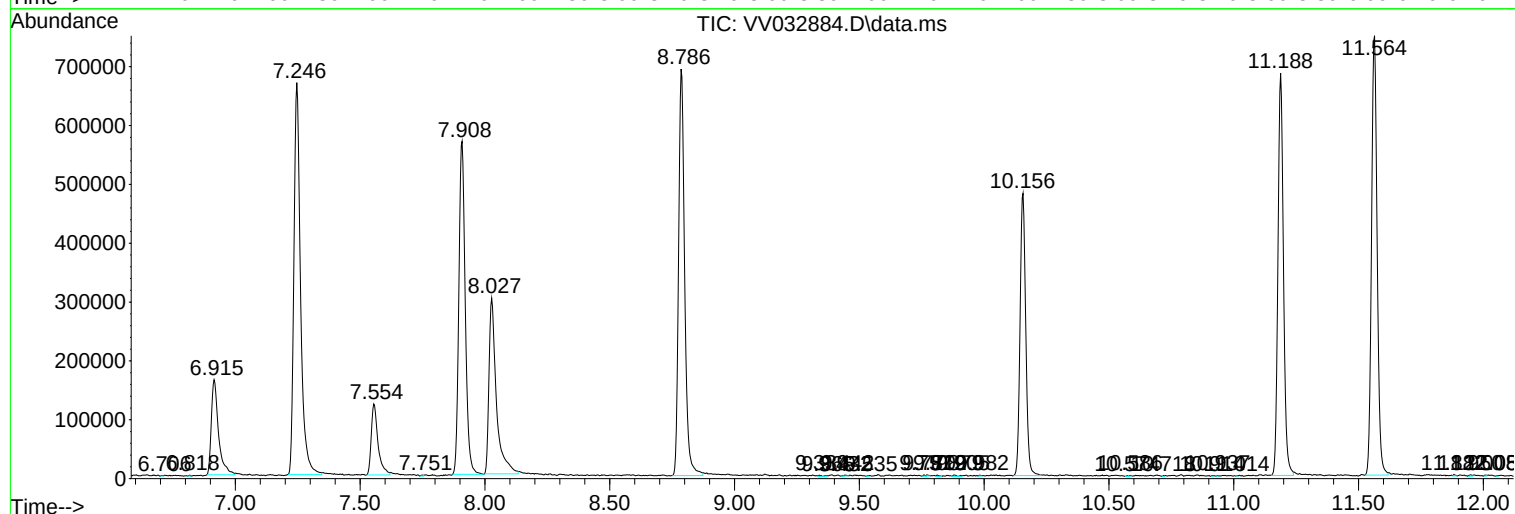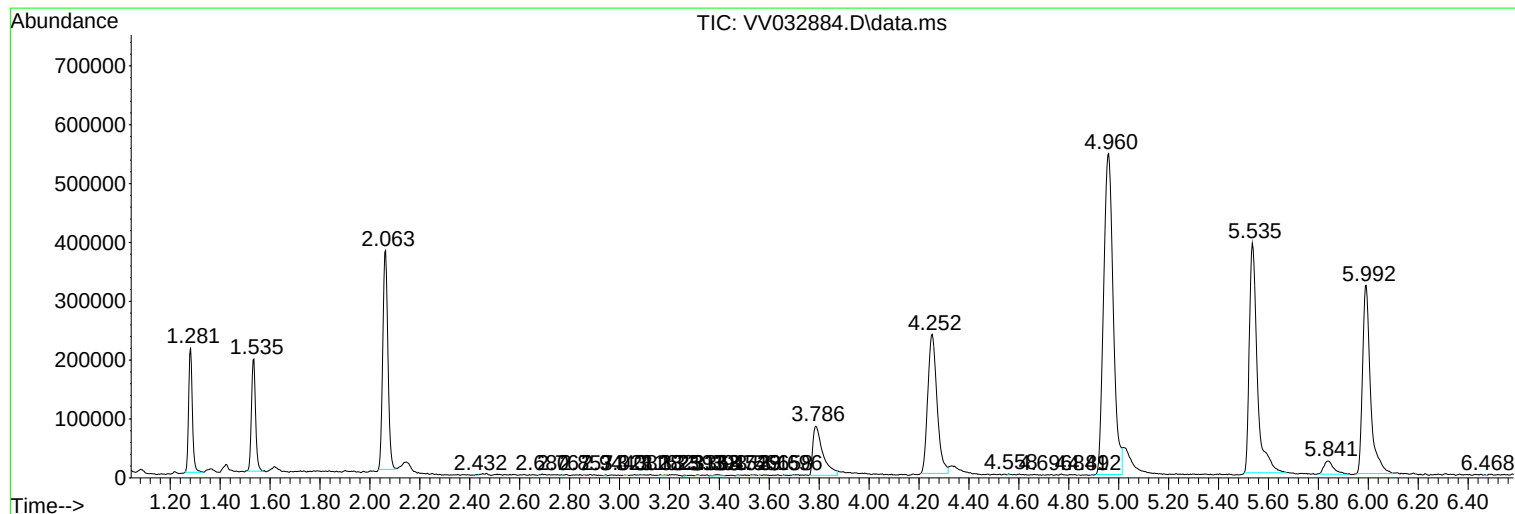

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032884.D
Acq On : 10 Nov 2023 12:11
Operator : SY/MD
Sample : 05326-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E45K1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032884.D
Acq On : 10 Nov 2023 12:11
Operator : SY/MD
Sample : 05326-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E45K1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------