

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032886.D
 Acq On : 10 Nov 2023 12:57
 Operator : SY/MD
 Sample : 05326-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E45K5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

Signal : TIC: VV032886.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.163	35	38	43	rBV6	2015	2136	0.14%	0.019%
2	1.281	69	75	89	rVB	206387	210773	13.81%	1.847%
3	1.532	147	153	163	rBV	175729	201872	13.22%	1.769%
4	2.063	309	318	332	rBV	361984	525619	34.43%	4.607%
5	2.365	411	412	416	rVB3	979	432	0.03%	0.004%
6	2.494	449	452	455	rBV5	2406	1745	0.11%	0.015%
7	2.558	467	472	476	rBV7	2245	2184	0.14%	0.019%
8	2.622	490	492	495	rVB3	1481	685	0.04%	0.006%
9	2.638	495	497	498	rBV2	1549	692	0.05%	0.006%
10	2.680	507	510	511	rVB3	1168	462	0.03%	0.004%
11	2.825	552	555	558	rBV4	1891	1279	0.08%	0.011%
12	2.860	563	566	570	rVB6	2214	1822	0.12%	0.016%
13	2.892	570	576	577	rBV6	844	729	0.05%	0.006%
14	2.947	590	593	598	rBV7	1109	974	0.06%	0.009%
15	2.986	603	605	609	rBV5	1262	737	0.05%	0.006%
16	3.056	624	627	628	rBV3	1523	864	0.06%	0.008%
17	3.156	656	658	663	rVB6	1211	805	0.05%	0.007%
18	3.185	663	667	671	rBV5	1289	1068	0.07%	0.009%
19	3.233	678	682	685	rVB5	1359	1149	0.08%	0.010%
20	3.269	691	693	698	rVB5	1255	1001	0.07%	0.009%
21	3.397	730	733	736	rBV4	1246	948	0.06%	0.008%
22	3.478	756	758	760	rBV3	1541	612	0.04%	0.005%
23	3.539	771	777	779	rBV7	1088	1049	0.07%	0.009%
24	3.674	816	819	821	rVB4	2039	1190	0.08%	0.010%
25	3.709	828	830	833	rVB4	1408	816	0.05%	0.007%
26	3.728	835	836	840	rBV4	1143	612	0.04%	0.005%
27	3.786	846	854	881	rBV	79715	218892	14.34%	1.919%
28	4.252	984	999	1020	rBV	230307	605075	39.64%	5.303%
29	4.748	1149	1153	1154	rBV4	1238	687	0.05%	0.006%
30	4.825	1174	1177	1179	rBV4	1253	703	0.05%	0.006%
31	4.838	1179	1181	1183	rBV3	1368	765	0.05%	0.007%
32	4.960	1202	1219	1260	rBV2	536144	1526604	100.00%	13.380%
33	5.262	1311	1313	1315	rBV2	1757	963	0.06%	0.008%
34	5.535	1387	1398	1432	rBV	391541	879725	57.63%	7.711%
35	5.989	1528	1539	1571	rBV	307661	680730	44.59%	5.966%
36	6.420	1667	1673	1676	rVB8	1684	1840	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032886.D
 Acq On : 10 Nov 2023 12:57
 Operator : SY/MD
 Sample : 05326-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E45K5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

37	6.432	1676	1677	1678	rBV	1488	542	0.04%	0.005%
38	6.590	1721	1726	1729	rBV6	2510	1974	0.13%	0.017%
39	6.693	1754	1758	1759	rBV3	1201	805	0.05%	0.007%
40	6.834	1799	1802	1803	rBV3	1716	929	0.06%	0.008%
41	6.915	1817	1827	1850	rBV	157750	311144	20.38%	2.727%
42	7.169	1904	1906	1908	rBV3	2185	1174	0.08%	0.010%
43	7.246	1918	1930	1953	rBV	637454	1179681	77.27%	10.340%
44	7.555	2017	2026	2046	rBV	114661	216839	14.20%	1.901%
45	7.908	2128	2136	2150	rVB3	70857	122728	8.04%	1.076%
46	8.027	2164	2173	2212	rBV	286656	589819	38.64%	5.170%
47	8.474	2308	2312	2315	rBV5	2327	2274	0.15%	0.020%
48	8.542	2331	2333	2336	rBV4	1565	1226	0.08%	0.011%
49	8.786	2398	2409	2434	rBV	676590	1143786	74.92%	10.025%
50	9.207	2538	2540	2542	rBV3	967	456	0.03%	0.004%
51	9.333	2577	2579	2582	rBV4	1063	594	0.04%	0.005%
52	9.378	2591	2593	2599	rVB6	1353	717	0.05%	0.006%
53	9.519	2635	2637	2640	rBV4	1834	1048	0.07%	0.009%
54	9.551	2645	2647	2649	rBV3	1747	922	0.06%	0.008%
55	9.596	2660	2661	2664	rVB3	936	437	0.03%	0.004%
56	9.622	2664	2669	2670	rBV5	2055	1728	0.11%	0.015%
57	9.812	2726	2728	2731	rBV4	1229	786	0.05%	0.007%
58	10.005	2786	2788	2790	rBV3	1208	571	0.04%	0.005%
59	10.156	2824	2835	2857	rBV	459386	732048	47.95%	6.416%
60	10.265	2867	2869	2873	rBV5	1389	877	0.06%	0.008%
61	10.419	2916	2917	2919	rBV2	1284	520	0.03%	0.005%
62	10.471	2931	2933	2935	rBV3	1263	505	0.03%	0.004%
63	10.574	2963	2965	2968	rBV4	1920	1098	0.07%	0.010%
64	10.648	2984	2988	2991	rBV5	1485	1150	0.08%	0.010%
65	10.680	2995	2998	2999	rBV3	1248	785	0.05%	0.007%
66	10.709	3005	3007	3010	rVB3	1702	762	0.05%	0.007%
67	10.728	3010	3013	3014	rBV2	1468	778	0.05%	0.007%
68	10.754	3018	3021	3022	rVB3	1516	679	0.04%	0.006%
69	10.767	3022	3025	3026	rBV3	893	458	0.03%	0.004%
70	10.821	3040	3042	3046	rVB4	1682	1005	0.07%	0.009%
71	10.863	3049	3055	3057	rBV5	1893	1519	0.10%	0.013%
72	10.902	3064	3067	3070	rVB5	2020	1353	0.09%	0.012%
73	11.046	3110	3112	3114	rBV3	1496	826	0.05%	0.007%
74	11.085	3123	3124	3129	rVB4	2089	1121	0.07%	0.010%
75	11.120	3132	3135	3136	rBV3	2263	1124	0.07%	0.010%
76	11.188	3145	3156	3176	rBV	679576	1054786	69.09%	9.245%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
 Data File : VV032886.D
 Acq On : 10 Nov 2023 12:57
 Operator : SY/MD
 Sample : 05326-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E45K5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
 Title : VOC Analysis

77	11.564	3261	3273	3291	rBV	711709	1123738	73.61%	9.849%
78	12.066	3422	3429	3431	rBV7	2726	2654	0.17%	0.023%
79	12.175	3461	3463	3465	rBV3	1202	598	0.04%	0.005%
80	12.210	3470	3474	3479	rBV7	1019	1201	0.08%	0.011%
81	12.271	3489	3493	3495	rBV4	1406	1283	0.08%	0.011%
82	12.432	3541	3543	3545	rBV3	1120	541	0.04%	0.005%
83	12.448	3545	3548	3553	rBV6	1401	1162	0.08%	0.010%
84	12.474	3553	3556	3557	rBV3	1274	740	0.05%	0.006%
85	12.606	3595	3597	3600	rBV4	1813	802	0.05%	0.007%
86	12.657	3611	3613	3617	rVB3	2149	1211	0.08%	0.011%
87	12.677	3617	3619	3621	rBV3	1581	912	0.06%	0.008%
88	12.715	3625	3631	3633	rBV7	2090	2050	0.13%	0.018%
89	12.821	3661	3664	3667	rBV5	2090	1702	0.11%	0.015%
90	13.114	3752	3755	3757	rBV4	1108	740	0.05%	0.006%
91	13.278	3804	3806	3809	rBV4	1597	1182	0.08%	0.010%
92	13.320	3816	3819	3822	rBV5	1136	753	0.05%	0.007%
93	13.339	3822	3825	3827	rBV4	1481	949	0.06%	0.008%
94	13.416	3846	3849	3850	rBV3	1214	585	0.04%	0.005%
95	13.570	3894	3897	3904	rBV9	2106	2312	0.15%	0.020%
96	13.673	3928	3929	3931	rBV2	1605	771	0.05%	0.007%
97	14.049	4042	4046	4047	rBV3	2027	1266	0.08%	0.011%
98	14.175	4081	4085	4087	rBV4	1655	1117	0.07%	0.010%
99	14.185	4087	4088	4090	rBV2	1404	690	0.05%	0.006%
100	14.943	4322	4324	4327	rBV5	1133	652	0.04%	0.006%




Sum of corrected areas: 11409424

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032886.D
Acq On : 10 Nov 2023 12:57
Operator : SY/MD
Sample : 05326-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E45K5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

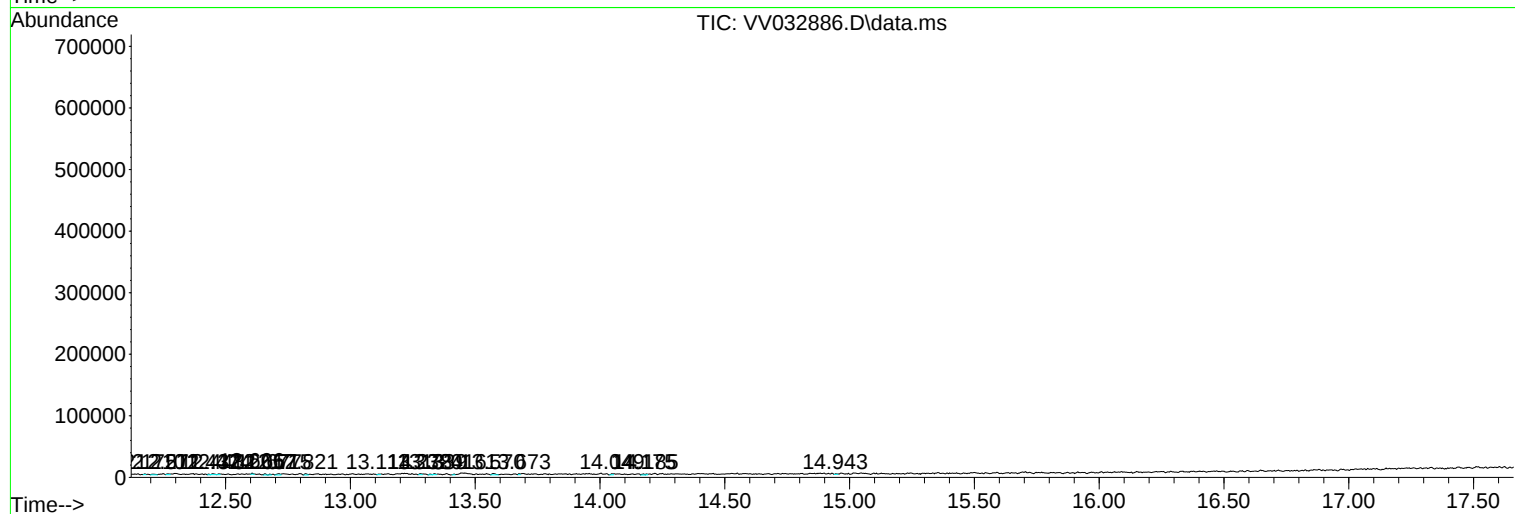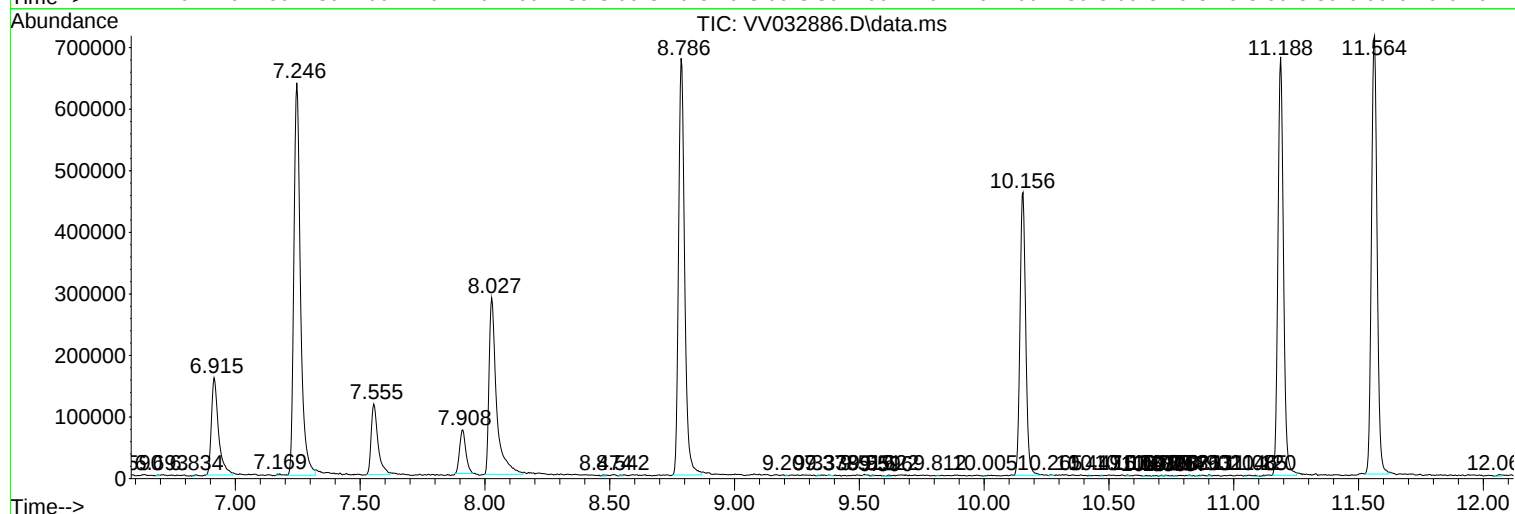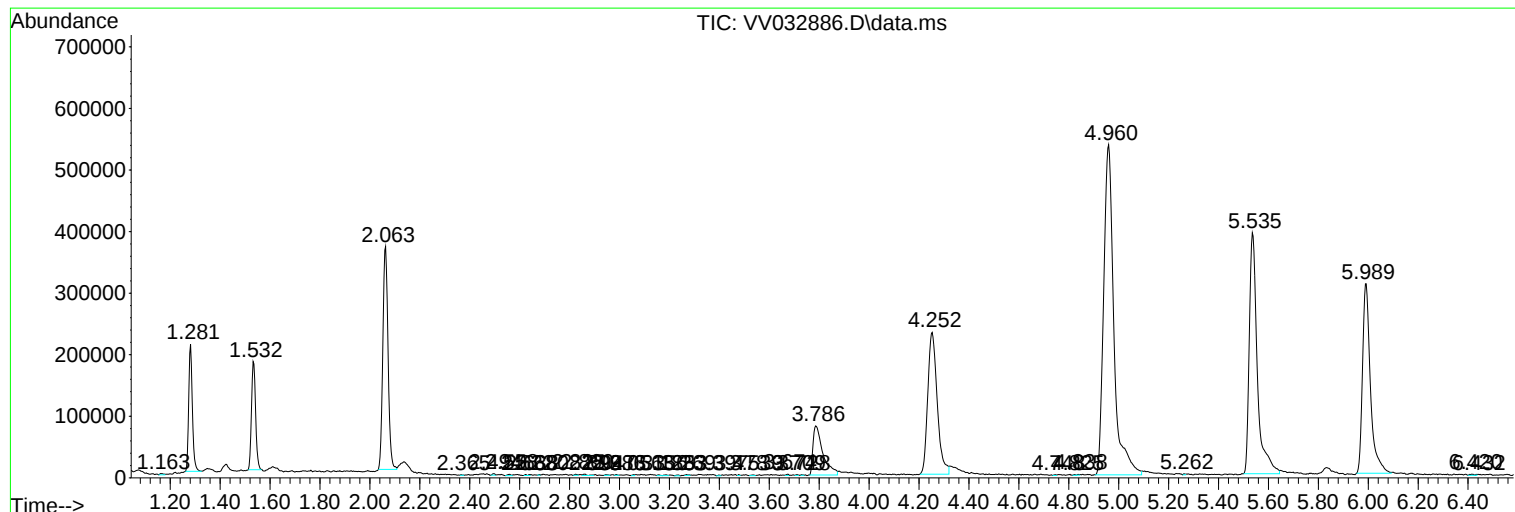

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032886.D
Acq On : 10 Nov 2023 12:57
Operator : SY/MD
Sample : 05326-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E45K5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111023\
Data File : VV032886.D
Acq On : 10 Nov 2023 12:57
Operator : SY/MD
Sample : 05326-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E45K5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM103123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------